
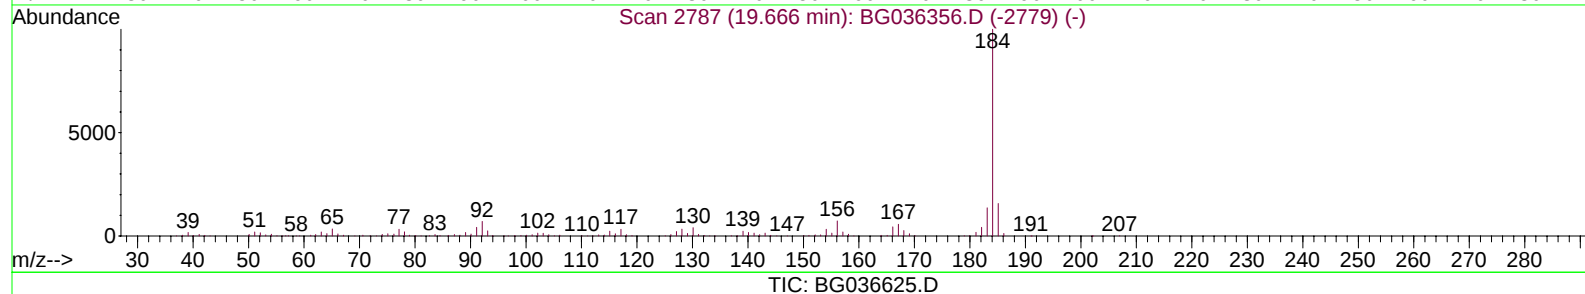
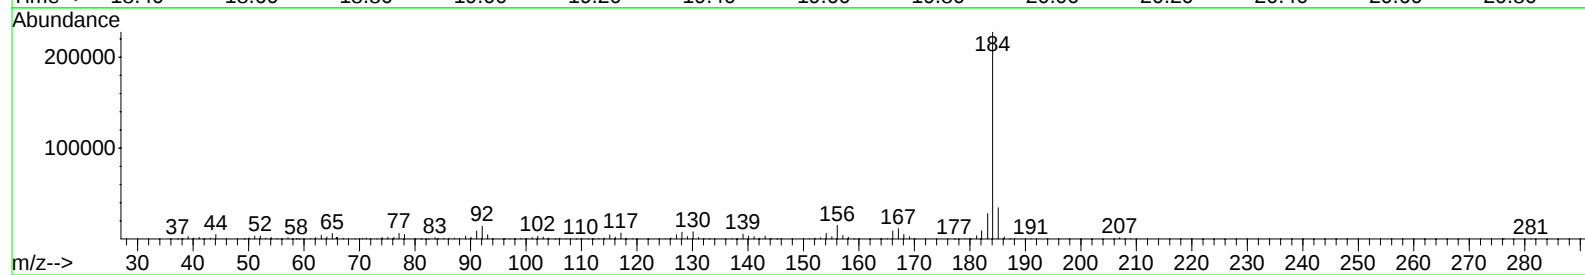


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091018\
Data File : BG036625.D
Acq On : 10 Sep 2018 15:10
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:31:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

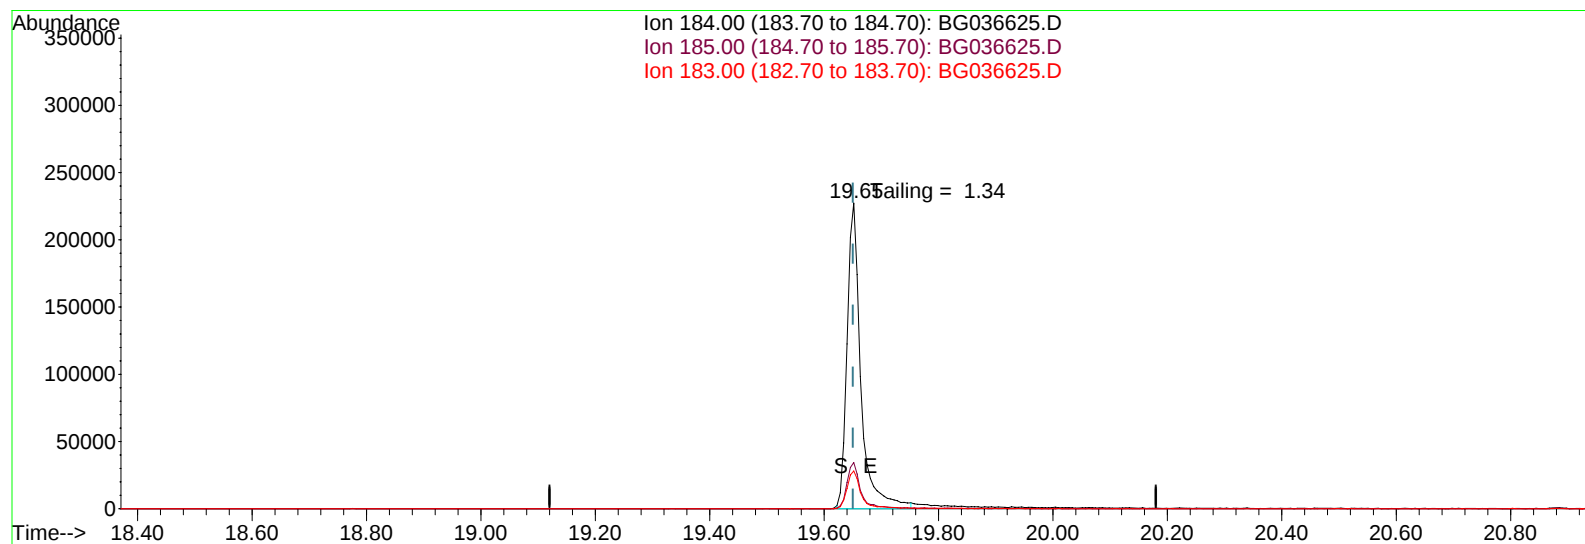

(76) Benzidine




19.652min (+0.002) 11203.11ng

response 398891

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.12
183.00	13.60	12.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091018\
Data File : BG036625.D
Acq On : 10 Sep 2018 15:10
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:31:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

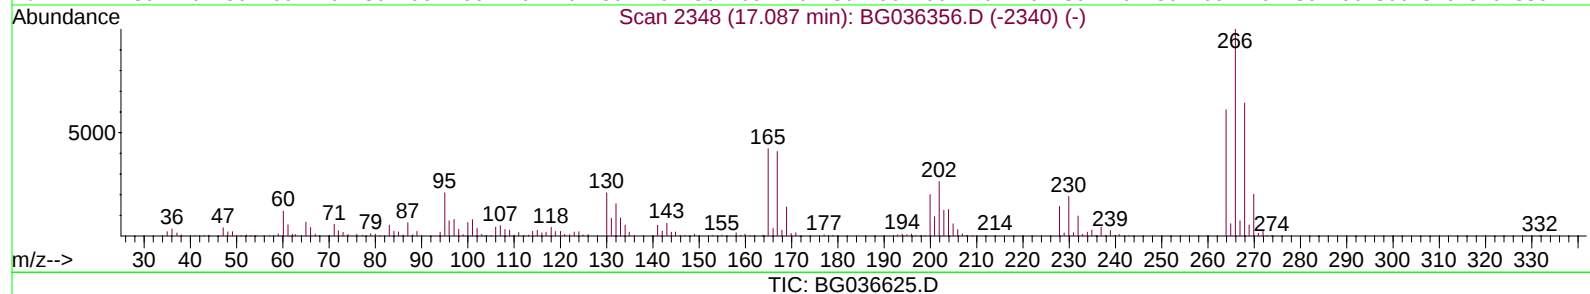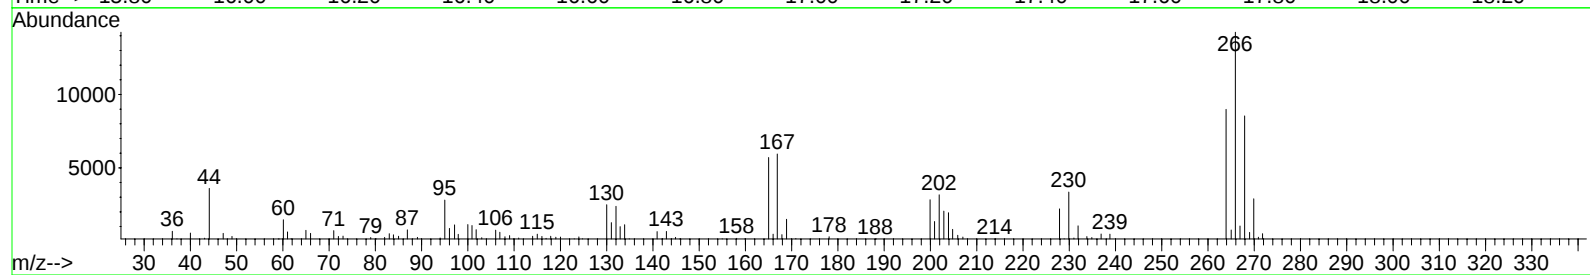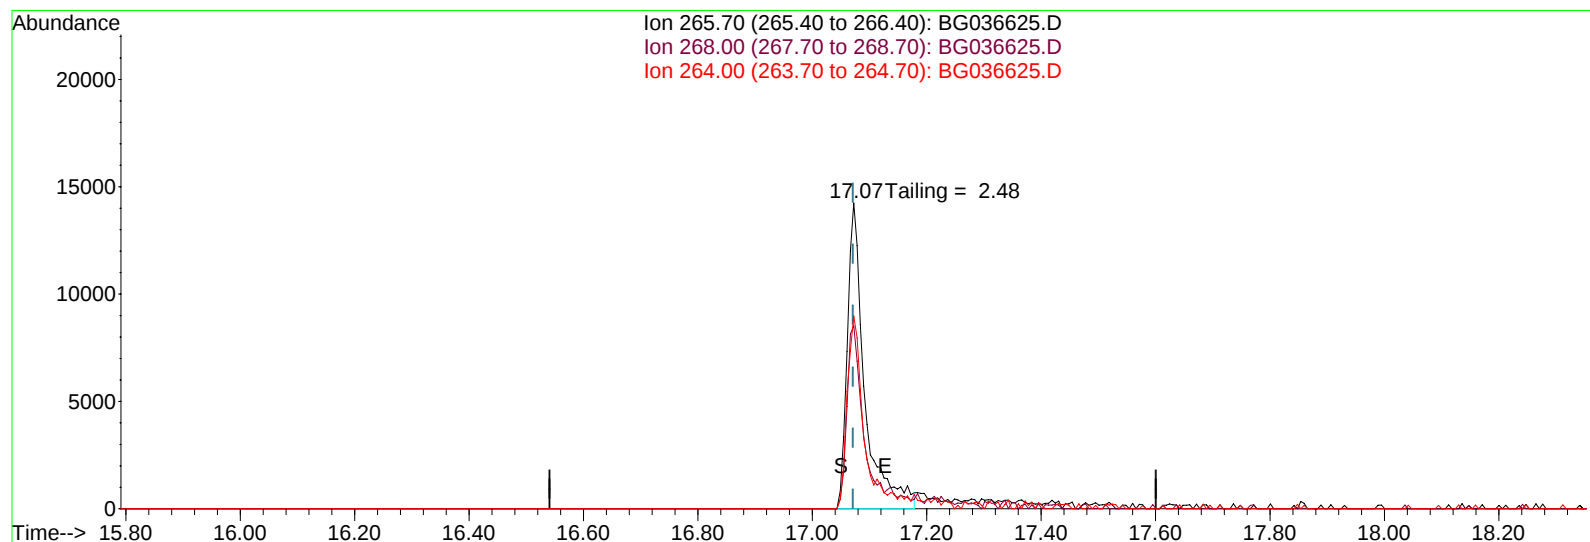

(69) Pentachlorophenol (C)

17.072min (+0.002) 64892.95ng

response 30624

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	59.95
264.00	61.10	63.06
0.00	0.00	0.00