
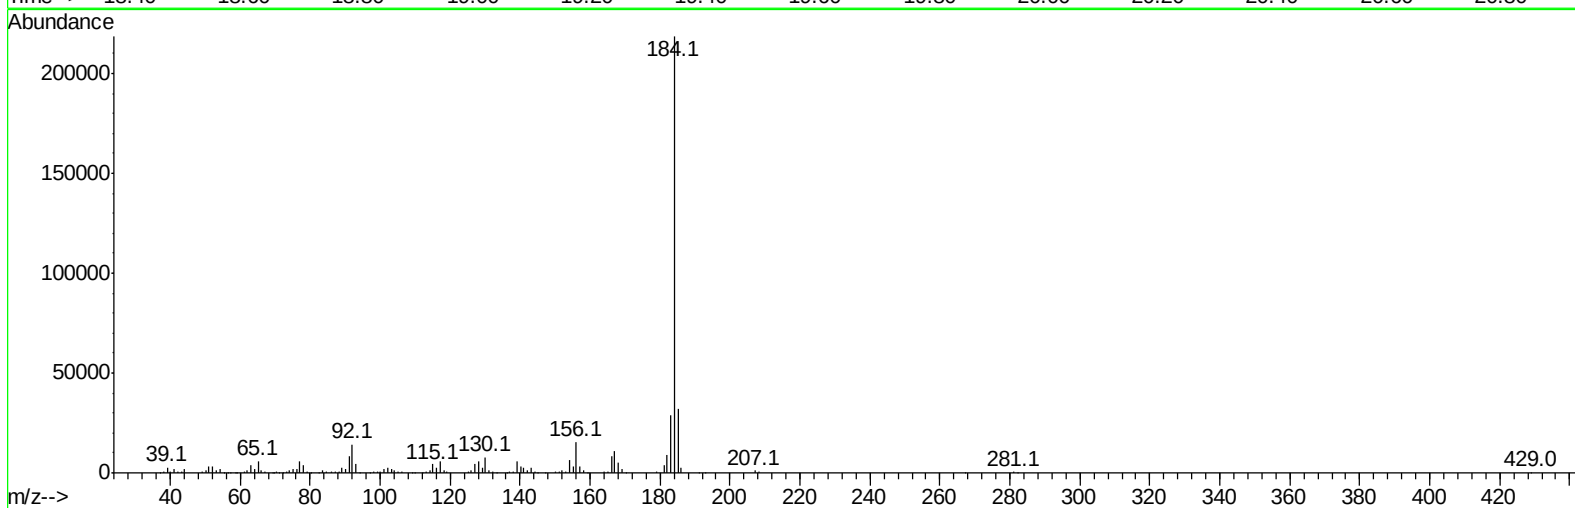


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091018\
Data File : BG036644.D
Acq On : 11 Sep 2018 3:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 09:20:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

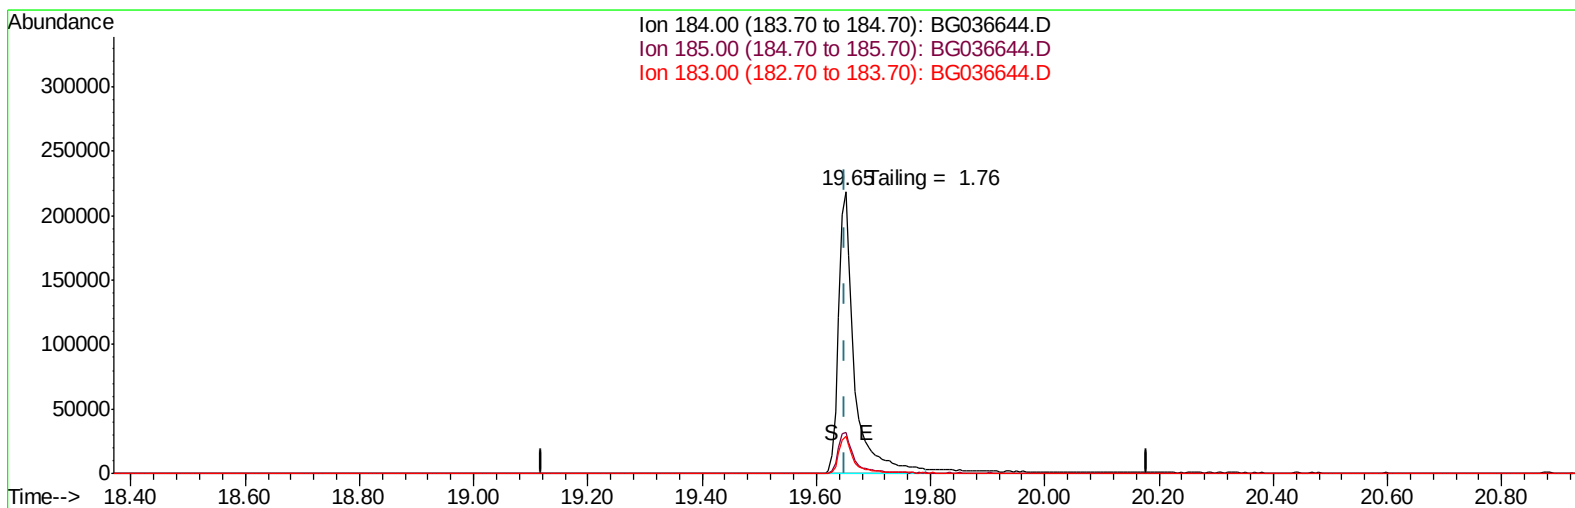

TIC: BG036644.D

(76) Benzidine



19.651min (+0.001) 118841.84ng

response 420866

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.76
183.00	13.60	13.24
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091018\
Data File : BG036644.D
Acq On : 11 Sep 2018 3:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 09:20:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

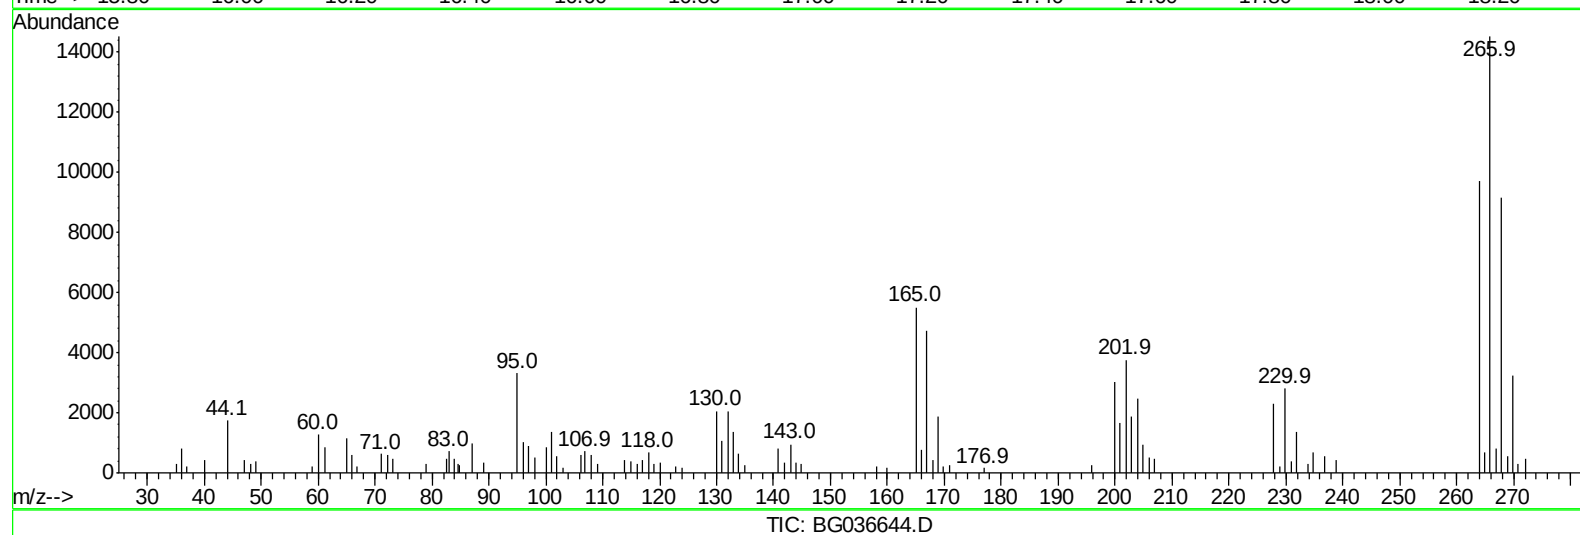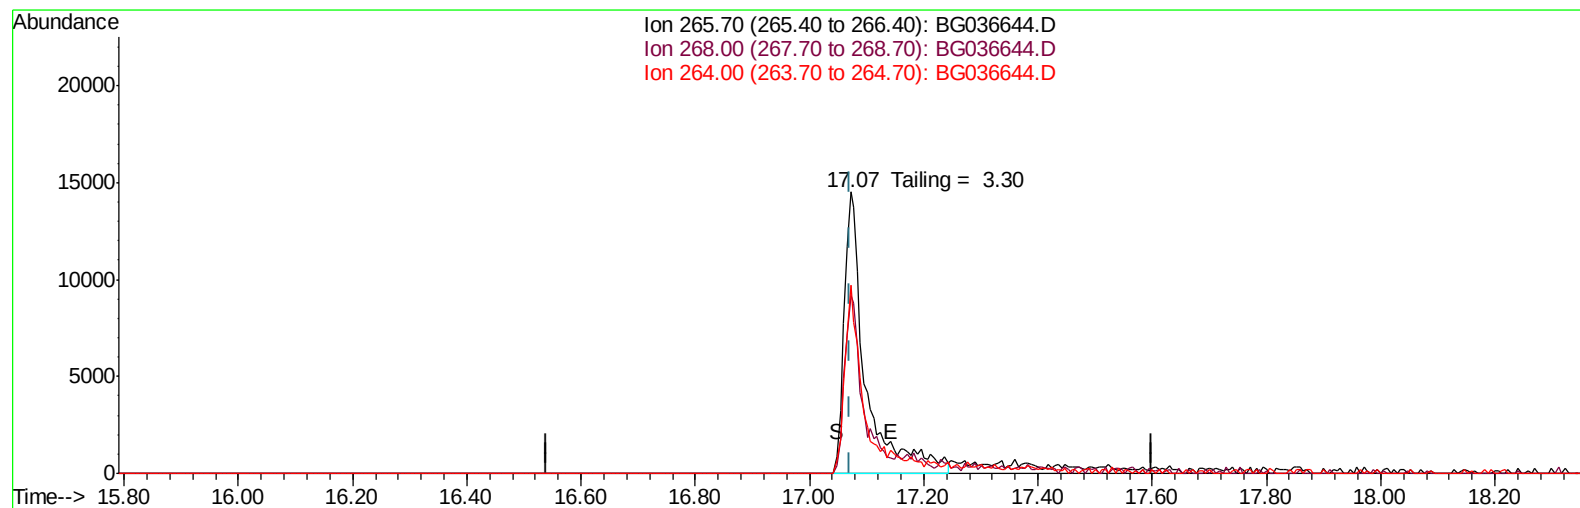

(69) Pentachlorophenol (C)

17.071min (+0.001) 24587.29ng

response 33409

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	63.06
264.00	61.10	66.75
0.00	0.00	0.00