

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091018\
 Data File : BG036649.D
 Acq On : 11 Sep 2018 6:42
 Operator : JU/SJ
 Sample : J4777-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-05-090718-E

Quant Time: Sep 11 07:38:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 31 13:03:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	56540	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	236733	20.00	ng	0.00
38) Acenaphthene-d10	14.68	164	152745	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	386888	20.00	ng	0.00
75) Chrysene-d12	21.69	240	397474	20.00	ng	0.00
86) Perylene-d12	24.90	264	302163	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	373551	104.80	ng	0.00
7) Phenol-d6	7.21	99	477699	93.61	ng	0.00
23) Nitrobenzene-d5	9.22	82	365676	83.81	ng	0.00
41) 2,4,6-Tribromophenol	16.17	330	193072	105.93	ng	0.00
44) 2-Fluorobiphenyl	13.30	172	840426	78.56	ng	-0.01
78) Terphenyl-d14	20.03	244	1453522	85.47	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091018\
Data File : BG036649.D
Acq On : 11 Sep 2018 6:42
Operator : JU/SJ
Sample : J4777-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-05-090718-E

Quant Time: Sep 11 07:38:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

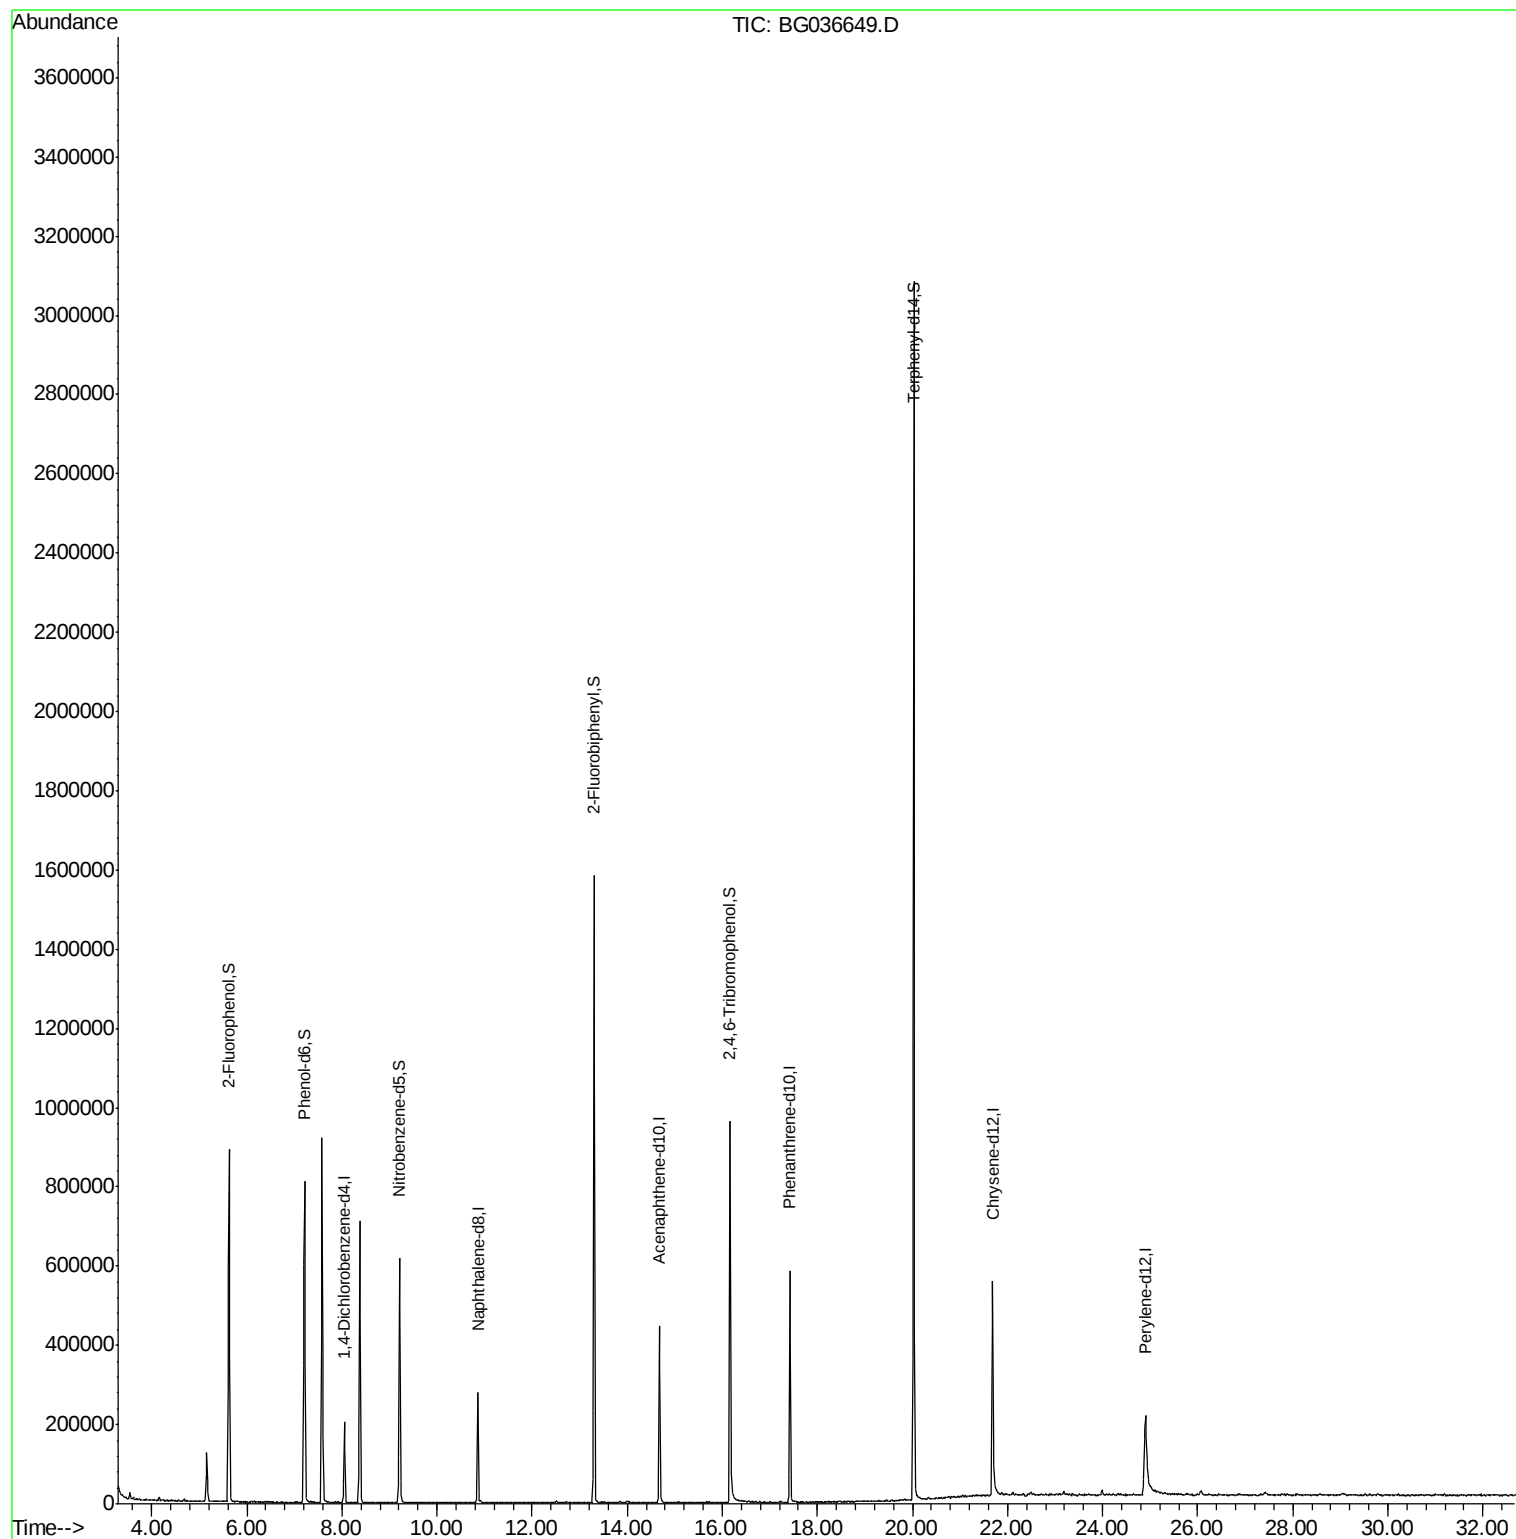

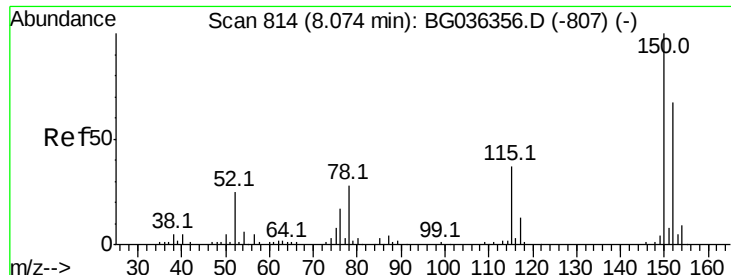


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 812
Delta R.T. -0.01 min
Lab File: BG036649.D
Acq: 11 Sep 2018 6:42

Instrument :
BNA_G
ClientSampleId :
PL-05-090718-E

Tot Ion	Ratio	Lower	Upper
152	100		
150	149.9	119.5	179.3
115	55.9	44.5	66.7

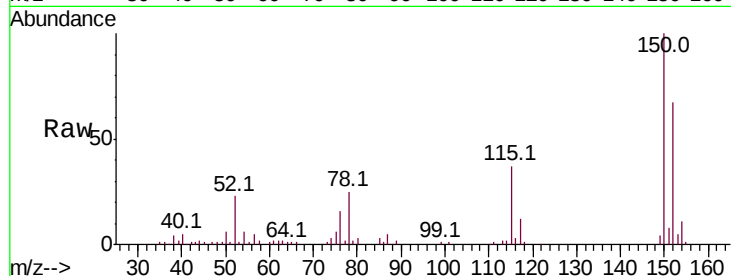


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

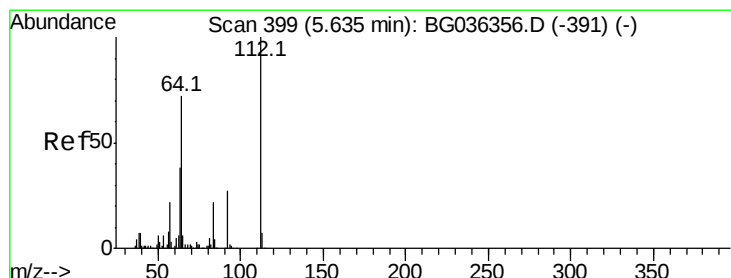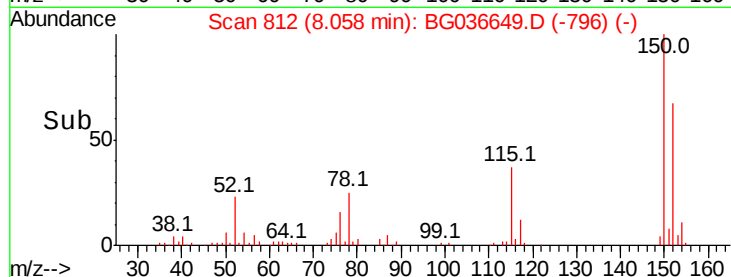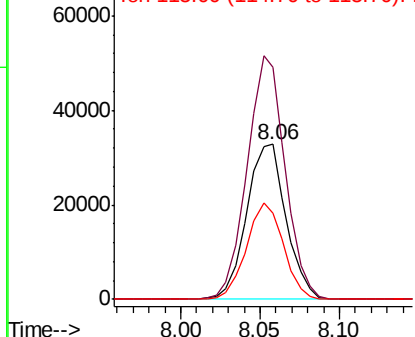



#5


2-Fluorophenol
Concen: 104.804 ng
RT: 5.63 min Scan# 398
Delta R.T. 0.00 min
Lab File: BG036649.D
Acq: 11 Sep 2018 6:42

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.9	57.2	85.8
63	36.1	30.8	46.2

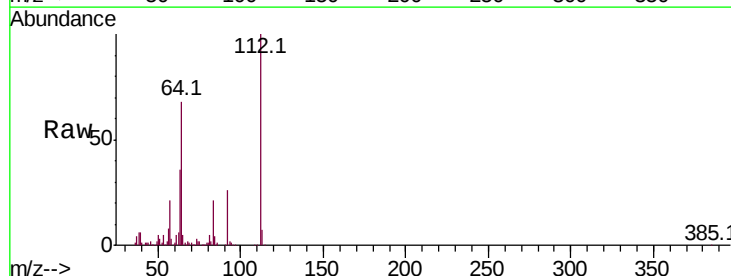

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

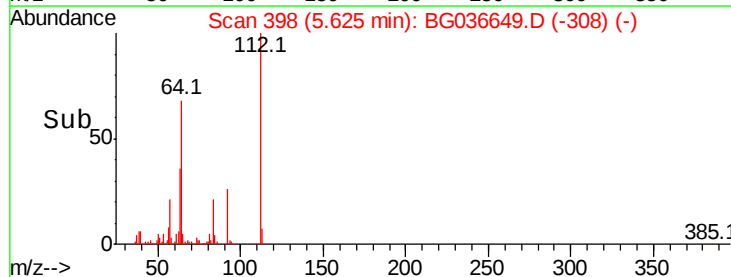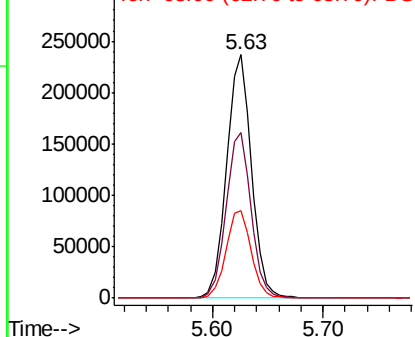

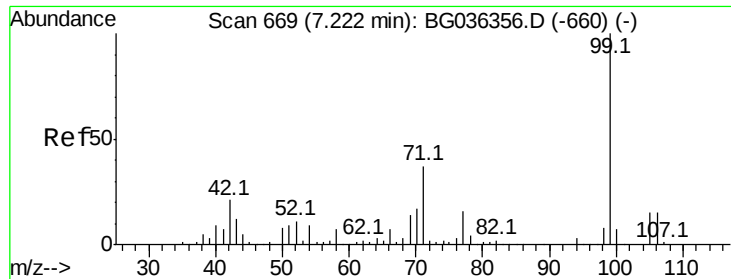

#7

Phenol-d6

Concen: 93.608 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG036649.D

Acq: 11 Sep 2018 6:42

Instrument :

BNA_G

ClientSampleId :

PL-05-090718-E


Tot Ion: 99 Resp: 477699

Ion Ratio Lower Upper




99 100

42 20.0 16.5 24.7

71 36.2 29.4 44.2

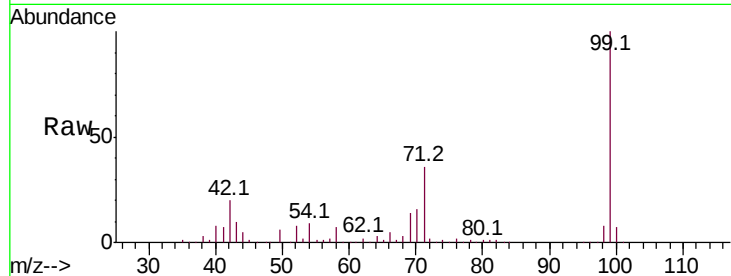

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

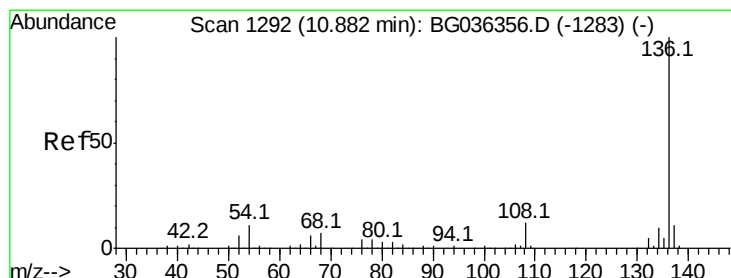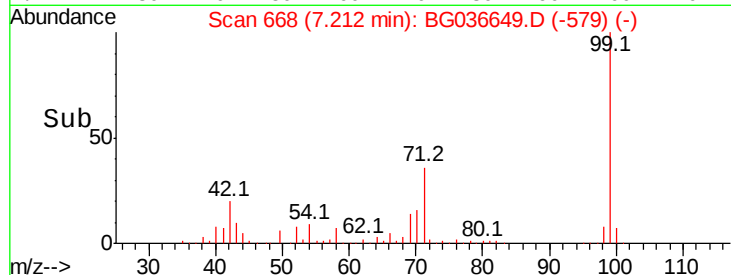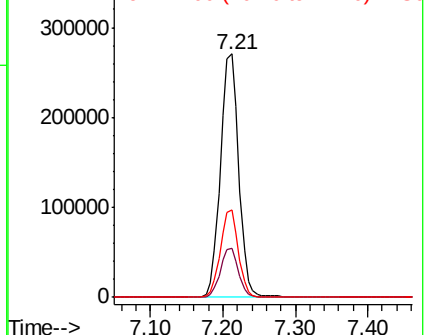

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.01 min

Lab File: BG036649.D

Acq: 11 Sep 2018 6:42

Tgt Ion: 136 Resp: 236733


Ion Ratio Lower Upper

136 100



137 11.3 8.8 13.2


54 10.1 9.2 13.8

68 6.3 5.8 8.6

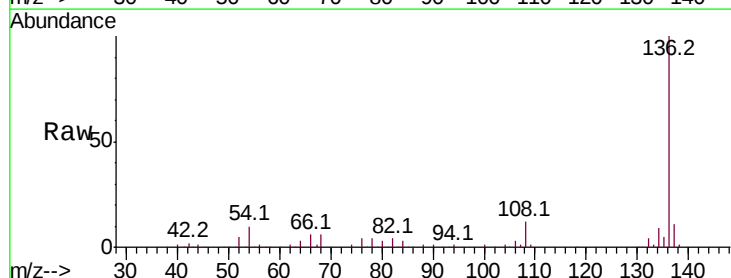

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



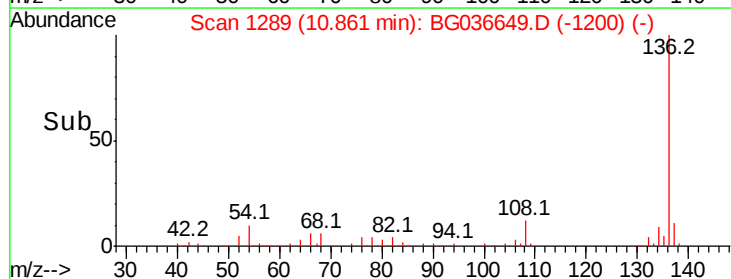
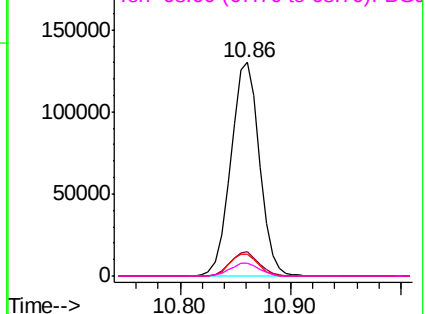


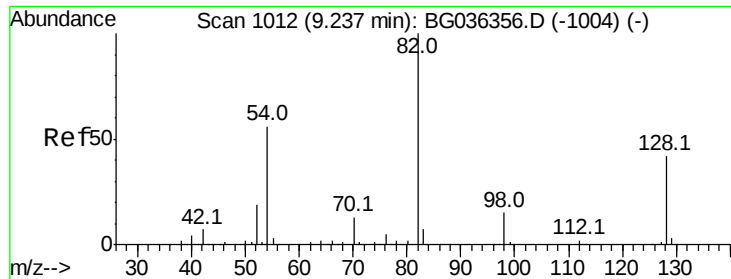

#23
 Nitrobenzene-d5
 Concen: 83.809 ng
 RT: 9.22 min Scan# 1009
 Delta R.T. -0.01 min
 Lab File: BG036649.D
 Acq: 11 Sep 2018 6:42




Instrument :
 BNA_G
 ClientSampleId :
 PL-05-090718-E


Tot Ion: 82 Resp: 365676
 Ion Ratio Lower Upper
 82 100
 128 42.9 33.3 49.9
 54 57.0 45.1 67.7

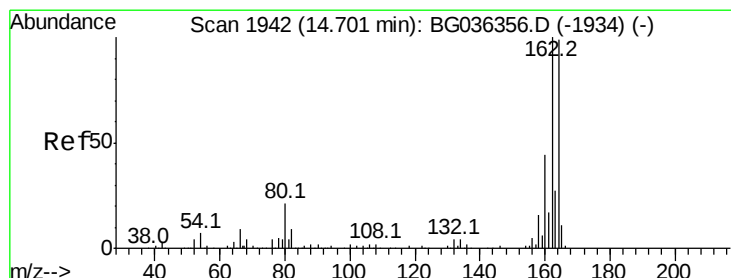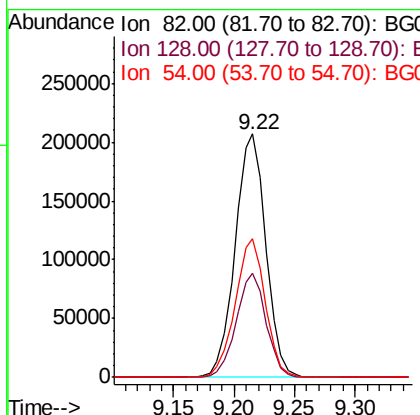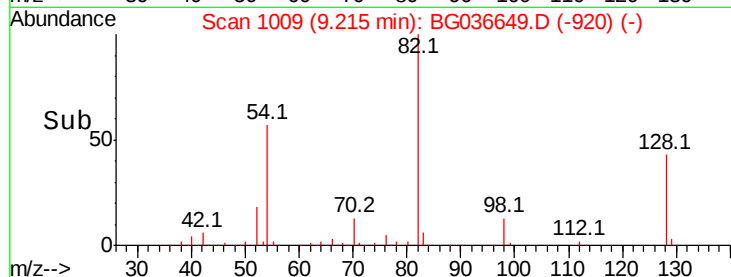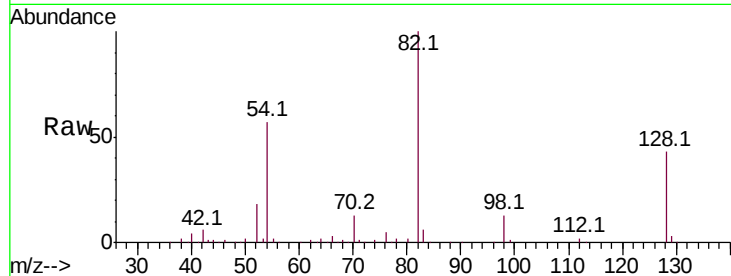

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1939
 Delta R.T. -0.01 min
 Lab File: BG036649.D
 Acq: 11 Sep 2018 6:42

Tgt Ion: 164 Resp: 152745
 Ion Ratio Lower Upper
 164 100
 162 106.2 80.7 121.1
 160 45.2 35.3 52.9

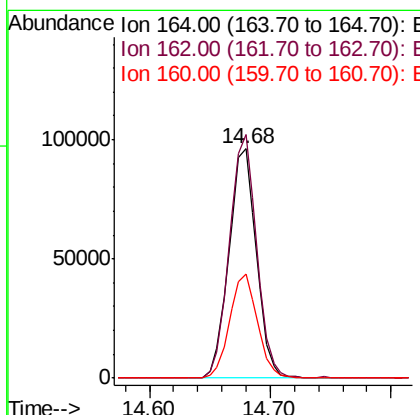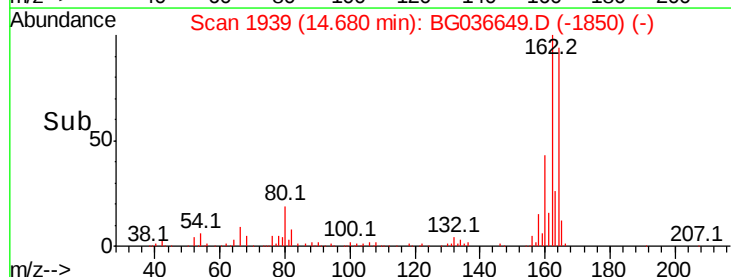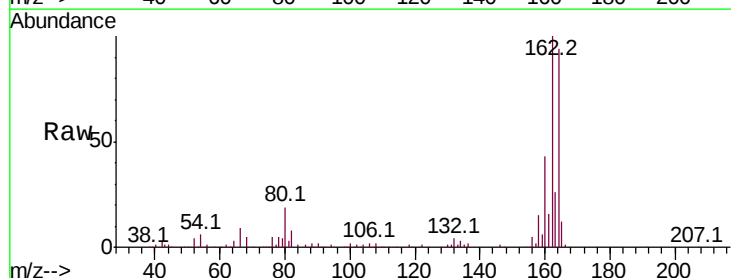


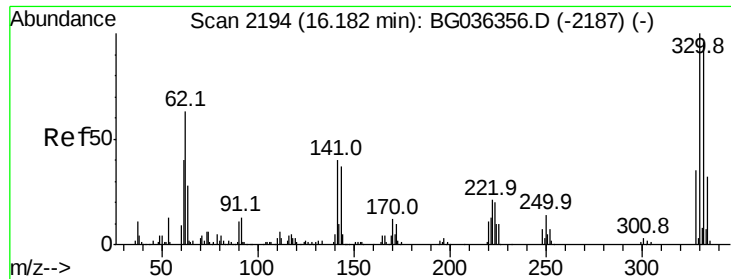

#41
 2,4,6-Tribromophenol
 Concen: 105.933 ng
 RT: 16.17 min Scan# 2192
 Delta R.T. -0.01 min
 Lab File: BG036649.D
 Acq: 11 Sep 2018 6:42

Instrument :
 BNA_G
 ClientSampleId :
 PL-05-090718-E

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.2	75.4	113.2
141	35.7	30.7	46.1



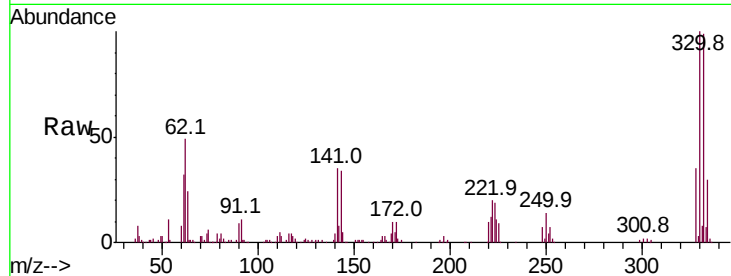


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

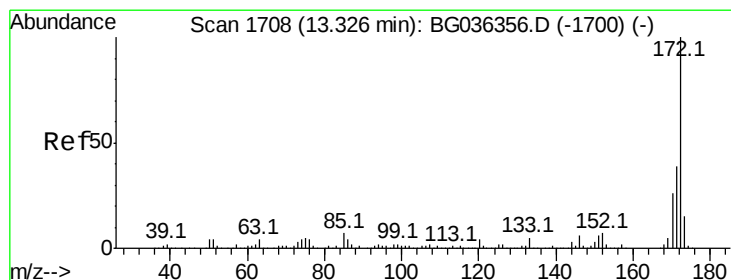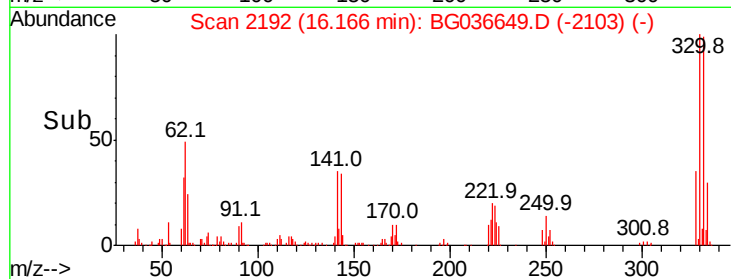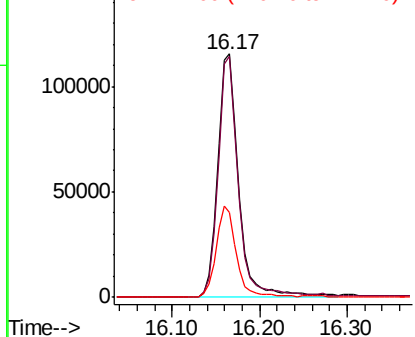

#44
 2-Fluorobiphenyl
 Concen: 78.561 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.01 min
 Lab File: BG036649.D
 Acq: 11 Sep 2018 6:42

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.3	31.3	46.9
170	25.5	21.0	31.6


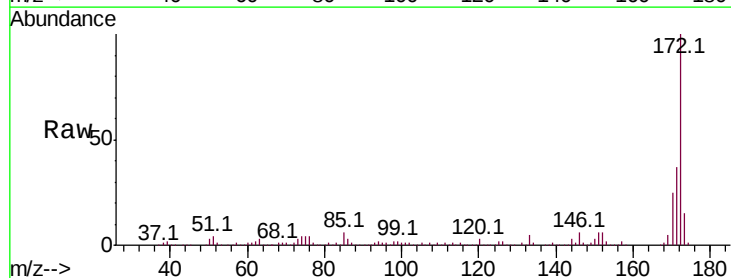



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



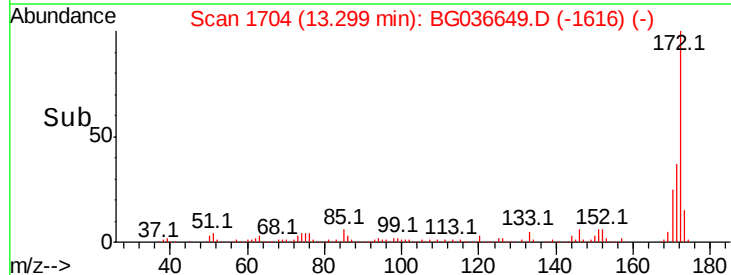
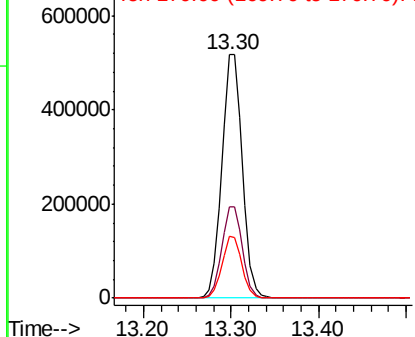


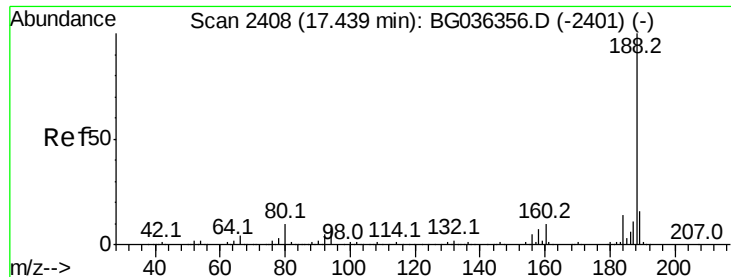

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2406
Delta R.T. -0.01 min
Lab File: BG036649.D
Acq: 11 Sep 2018 6:42




Instrument :
BNA_G
ClientSampleId :
PL-05-090718-E


Tot Ion:188 Resp: 386888
Ion Ratio Lower Upper
188 100
94 7.1 6.7 10.1
80 8.3 8.1 12.1

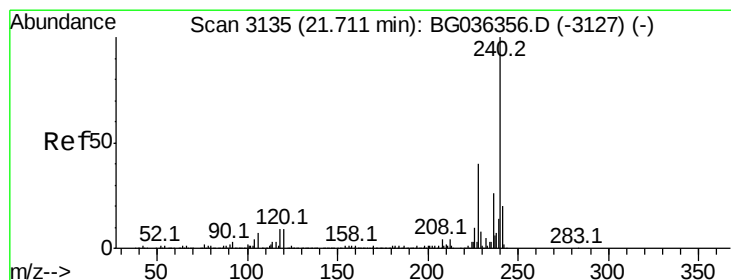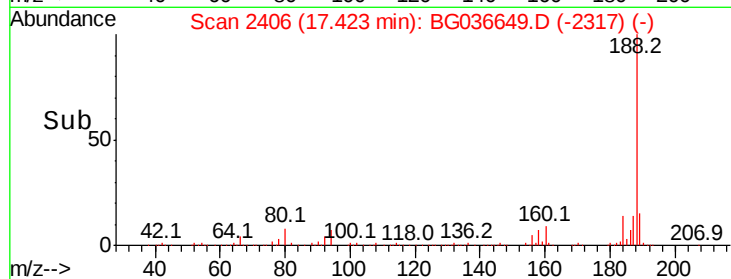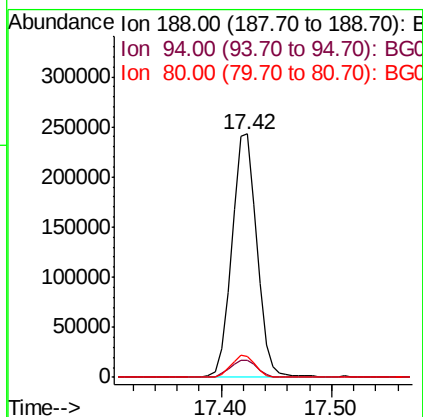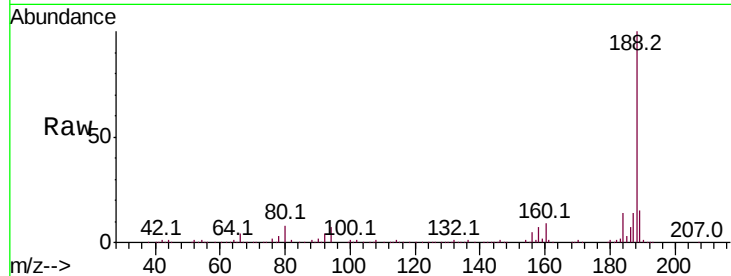

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.69 min Scan# 3132
Delta R.T. -0.01 min
Lab File: BG036649.D
Acq: 11 Sep 2018 6:42

Tgt Ion:240 Resp: 397474
Ion Ratio Lower Upper
240 100
120 7.7 6.9 10.3
236 26.2 21.2 31.8

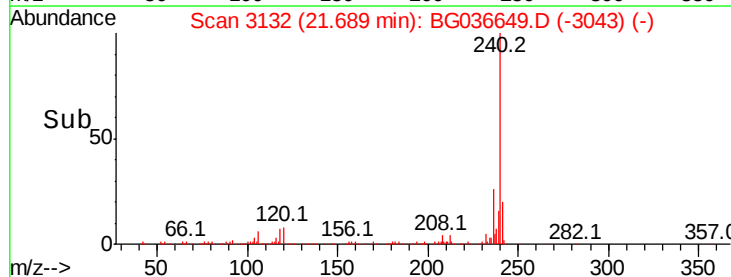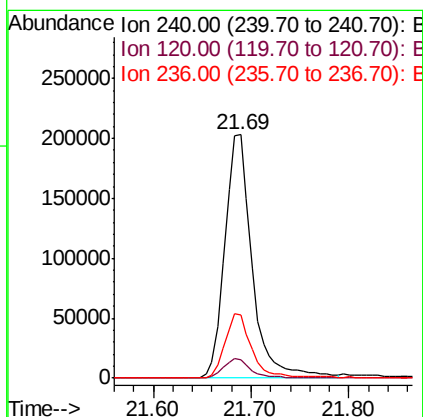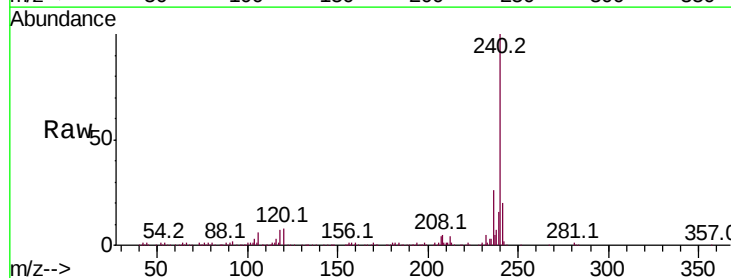

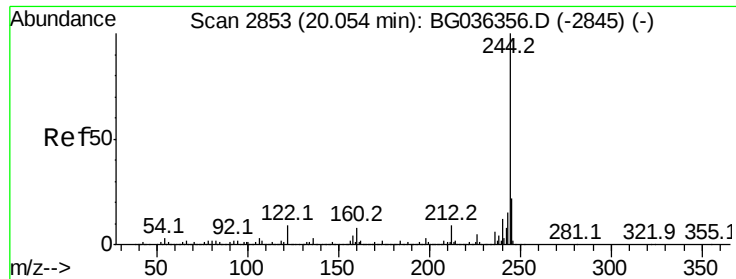

#78

Terphenyl-d14

Concen: 85.474 ng

RT: 20.03 min Scan# 2849

Delta R.T. -0.01 min

Lab File: BG036649.D

Acq: 11 Sep 2018 6:42

Instrument :

BNA_G

ClientSampleId :

PL-05-090718-E


Tot Ion:244 Resp: 1453522

Ion Ratio Lower Upper

244 100

212 9.1 7.0 10.6




122 8.8 7.1 10.7

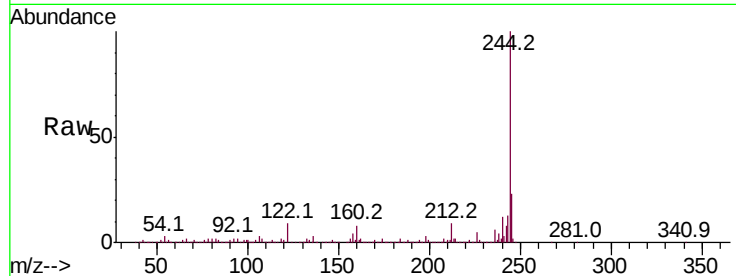

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

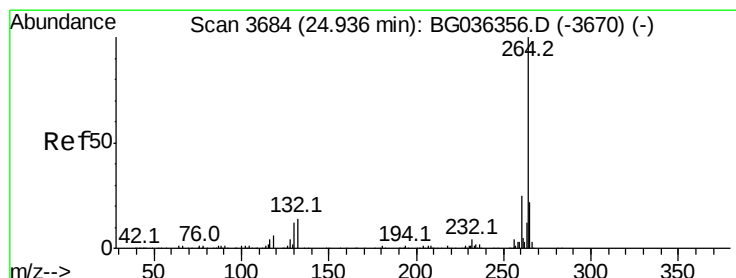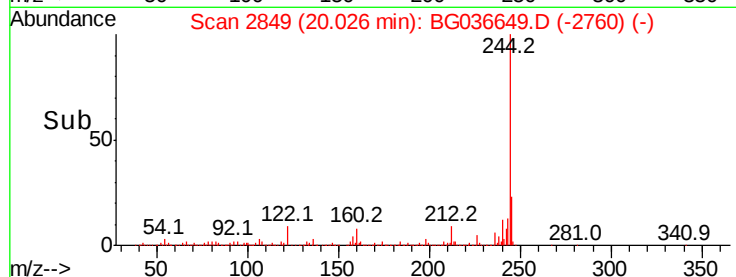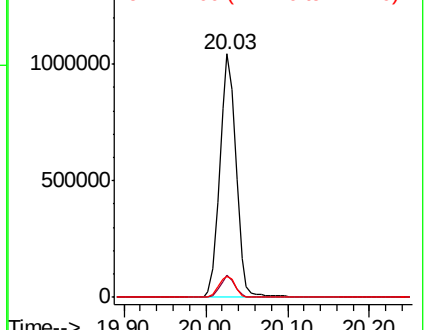

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.90 min Scan# 3678

Delta R.T. -0.01 min

Lab File: BG036649.D

Acq: 11 Sep 2018 6:42


Tgt Ion:264 Resp: 302163

Ion Ratio Lower Upper

264 100

260 22.8 19.6 29.4

265 21.9 17.4 26.0

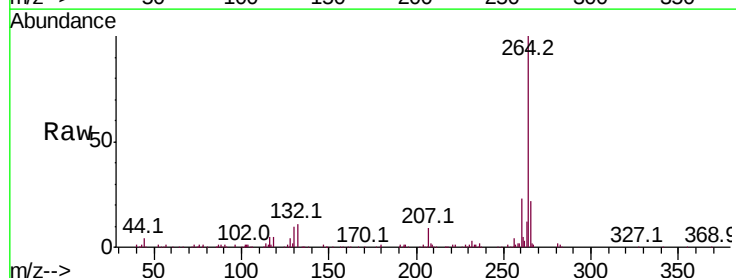

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

