


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091018\
 Data File : BG036625.D
 Acq On : 10 Sep 2018 15:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

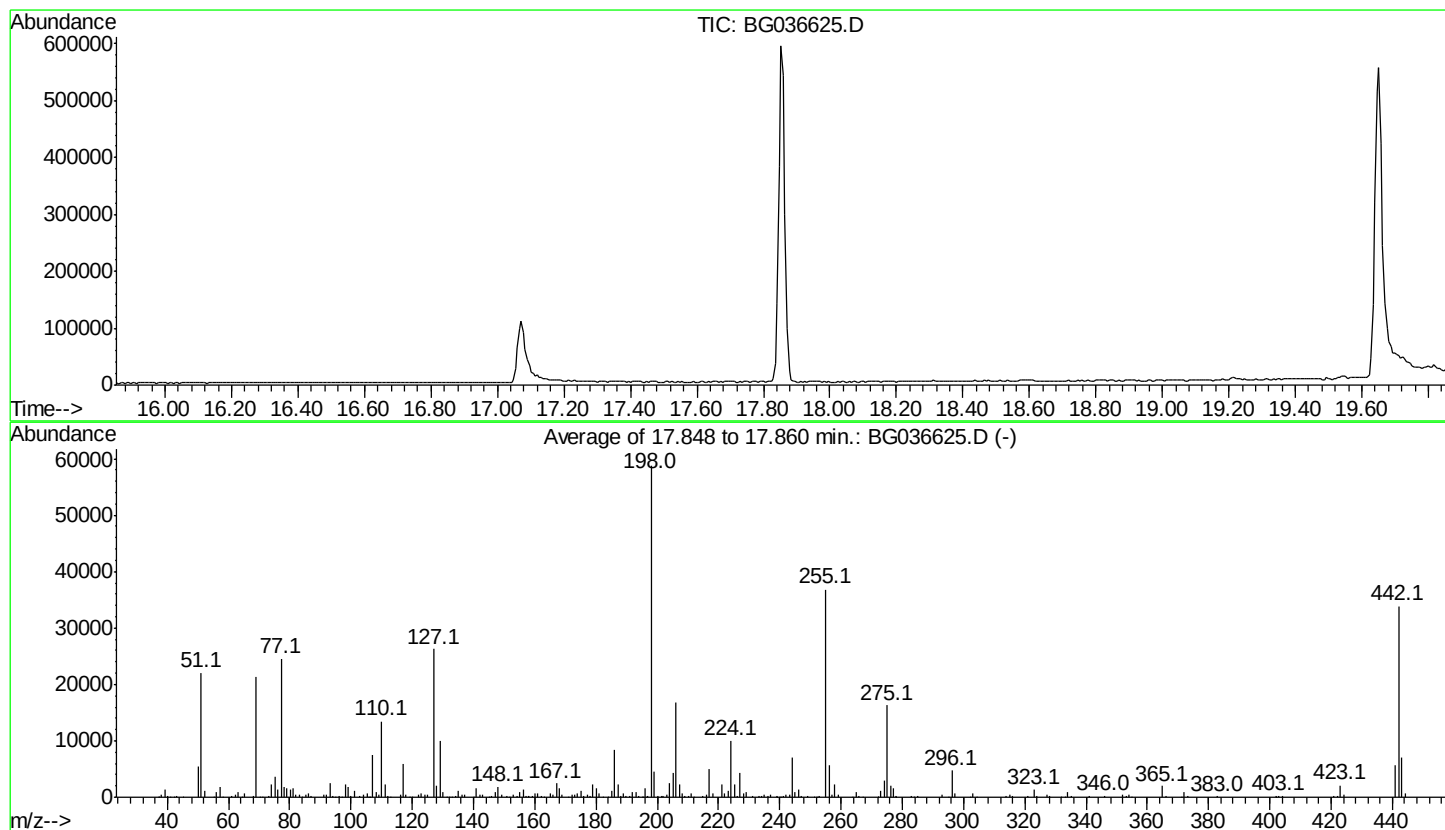

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	22034	PASS
68	69	0.00	2	1.2	257	PASS
69	198	0.00	100	36.3	21357	PASS
70	69	0.00	2	0.4	76	PASS
127	198	10	80	44.7	26269	PASS
197	198	0.00	2	0.4	249	PASS
198	198	100	100	100.0	58773	PASS
199	198	5	9	7.9	4616	PASS
275	198	10	60	27.7	16251	PASS
365	198	1	100	3.4	2007	PASS
441	198	0.01	100	9.5	5583	PASS
442	198	50	100	57.6	33856	PASS
443	442	15	24	20.5	6947	PASS