
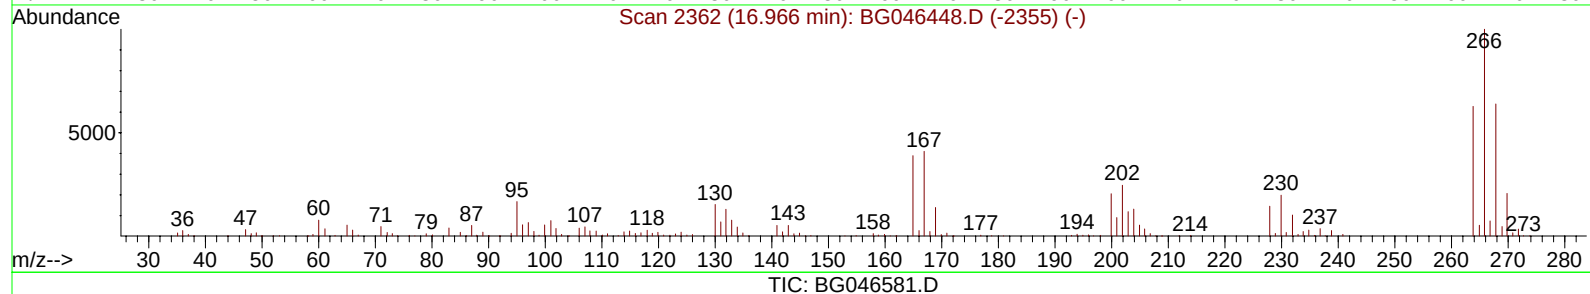
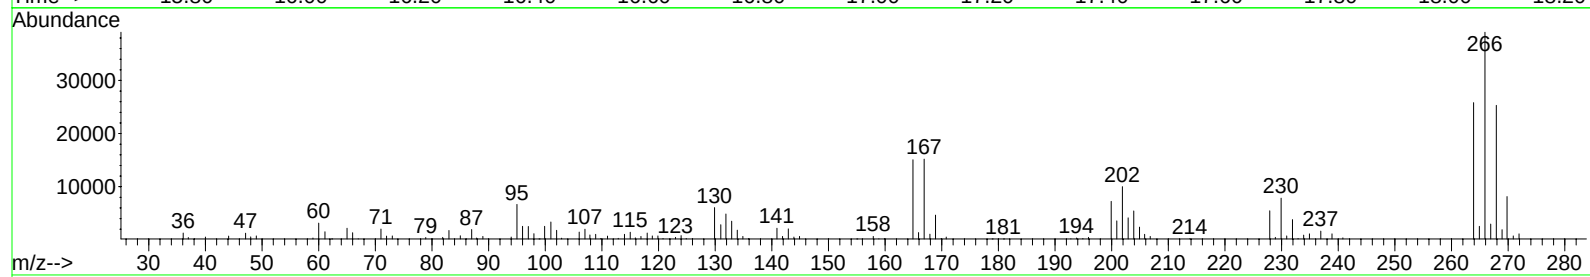


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091020\
Data File : BG046581.D
Acq On : 10 Sep 2020 11:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:53:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

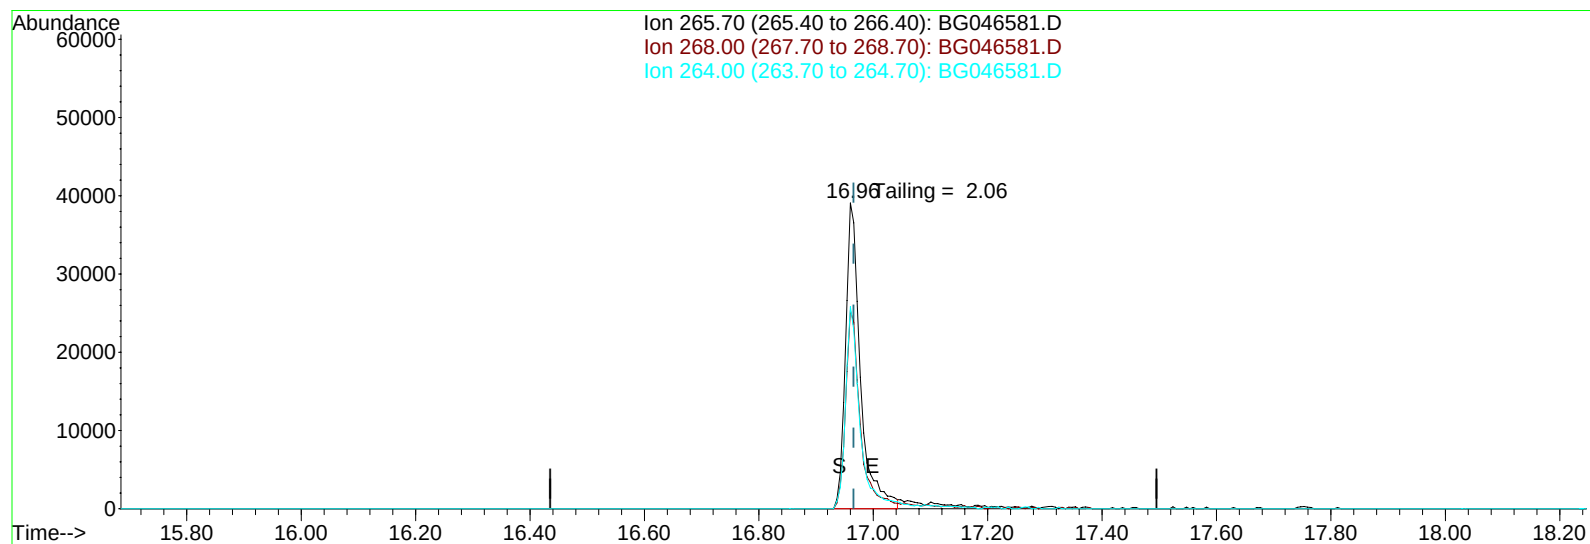

(70) Pentachlorophenol (C)




16.960min (-0.005) 158289.21ng

response 73732

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.81
264.00	62.70	66.08
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091020\
Data File : BG046581.D
Acq On : 10 Sep 2020 11:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:53:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

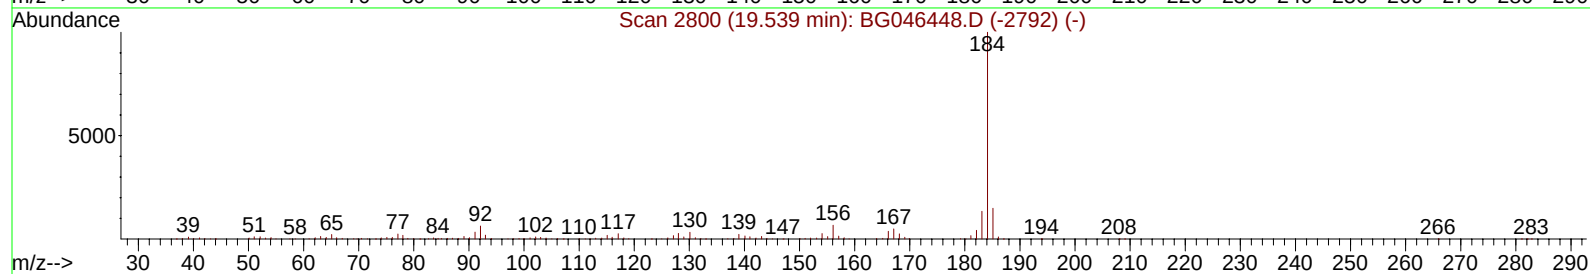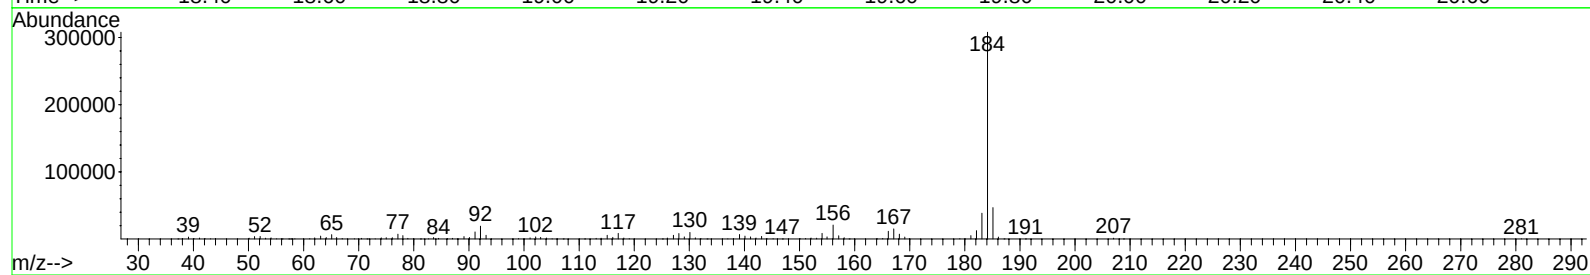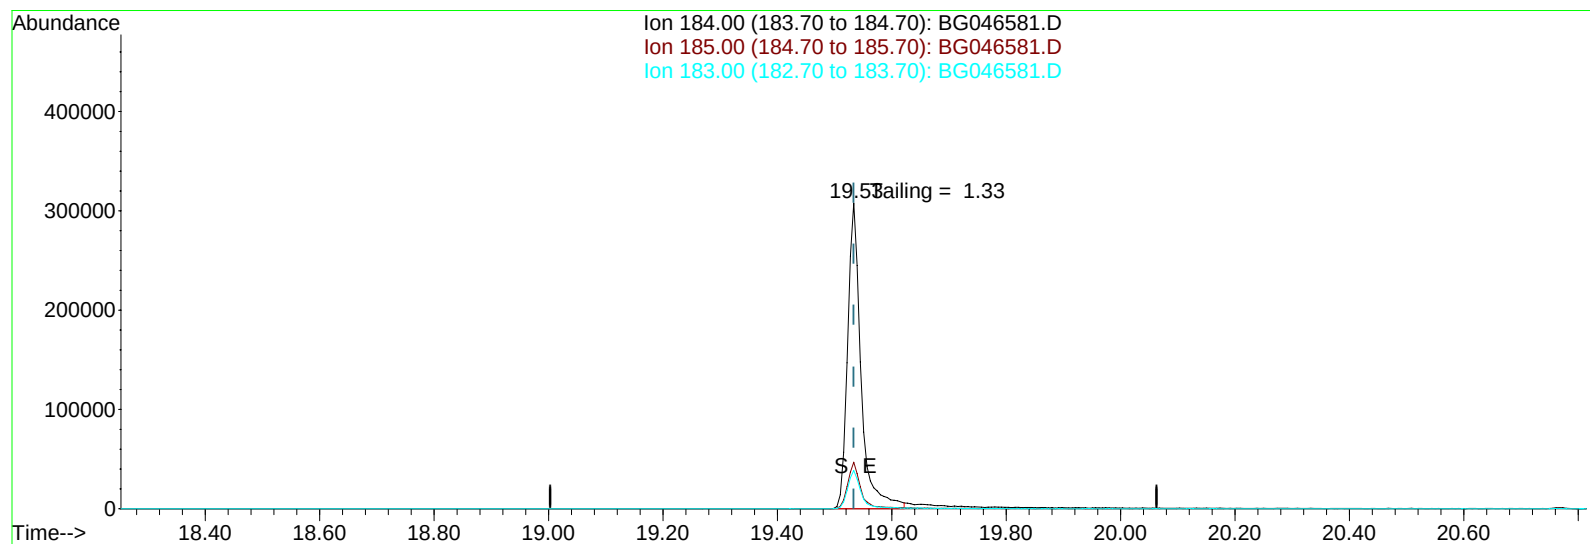

TIC: BG046581.D

(77) Benzidine

19.533min (+0.000) 64437.49ng

response 513584

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.23
183.00	13.40	12.52
0.00	0.00	0.00