




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062719.D
Acq On : 11 Sep 2024 3:43
Operator : JU/RC
Sample : PB163242BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK242

Manual IntegrationsAPPROVED

Quant Time: Sep 11 04:33:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/12/2024
Supervised By :mohammad ahmed 09/13/2024

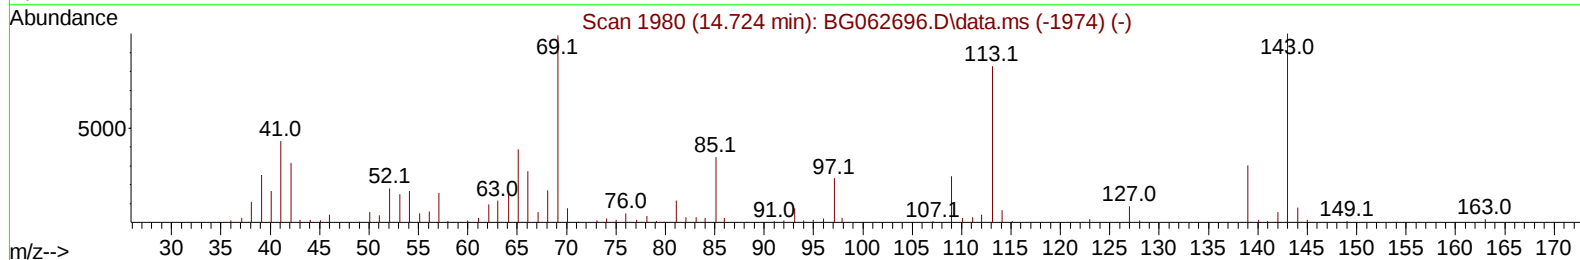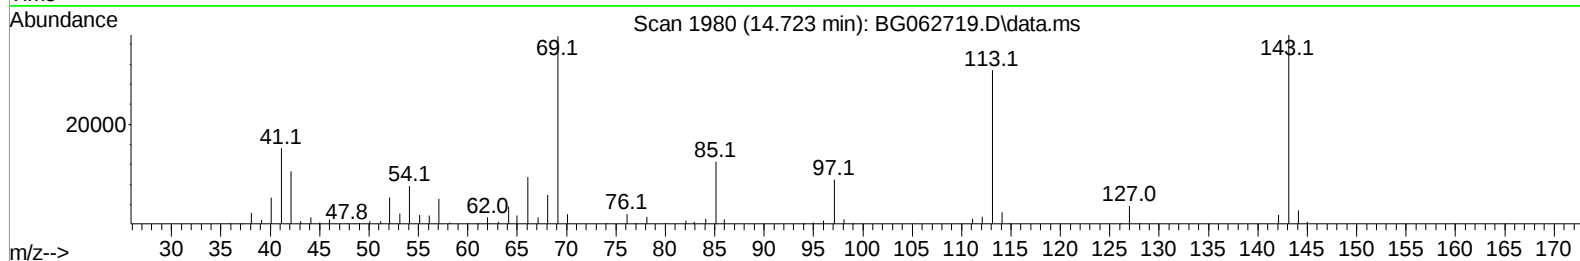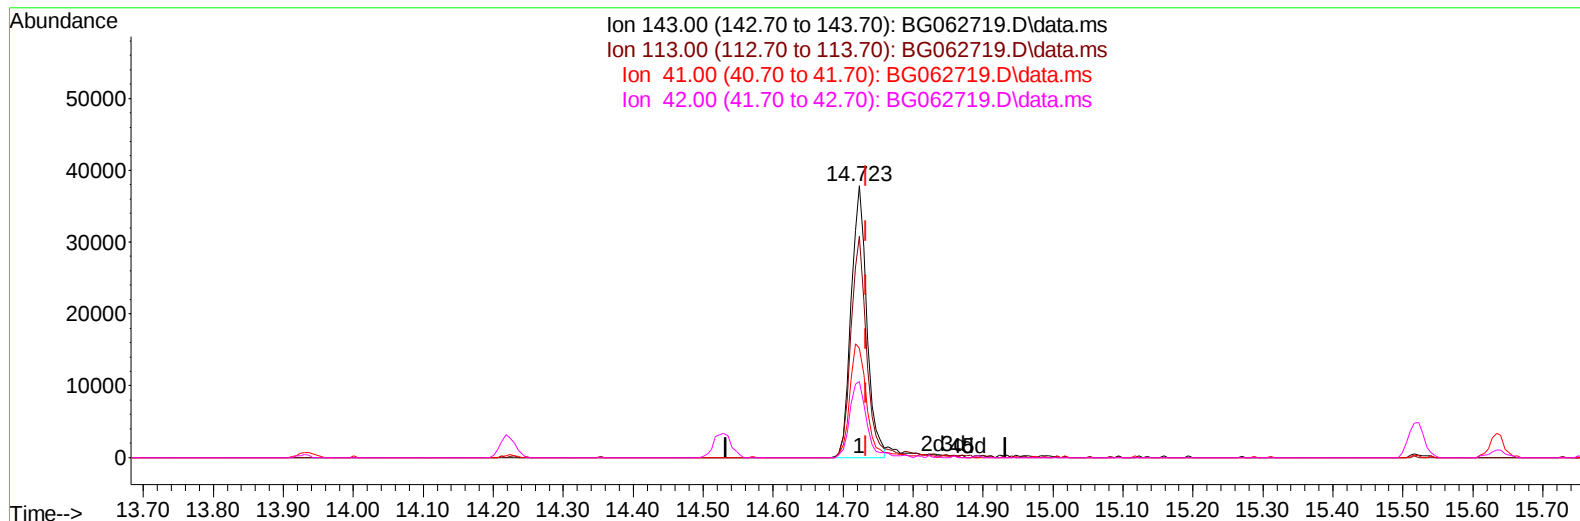

TIC: BG062719.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.723min (-0.009) 22.94 ng/u1

response 58362

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.40	81.38
41.00	45.80	40.20
42.00	31.60	28.01




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062719.D
Acq On : 11 Sep 2024 3:43
Operator : JU/RC
Sample : PB163242BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK242

Manual IntegrationsAPPROVED

Quant Time: Sep 11 04:33:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/12/2024
Supervised By :mohammad ahmed 09/13/2024

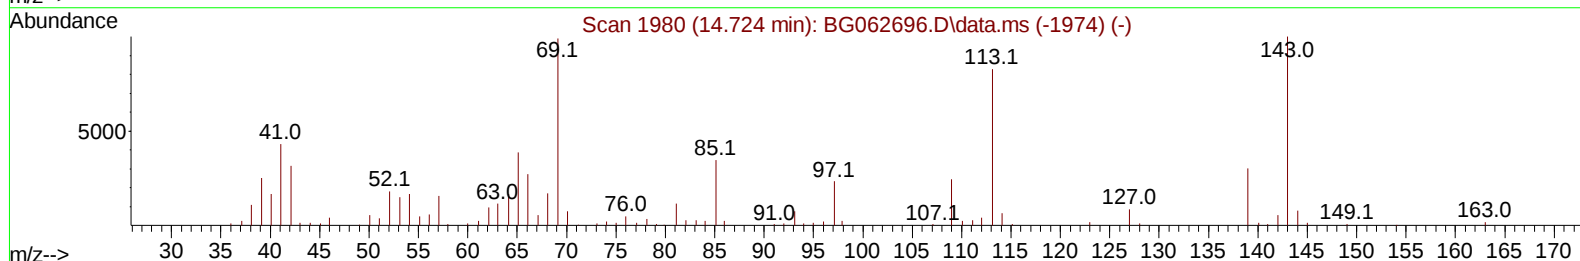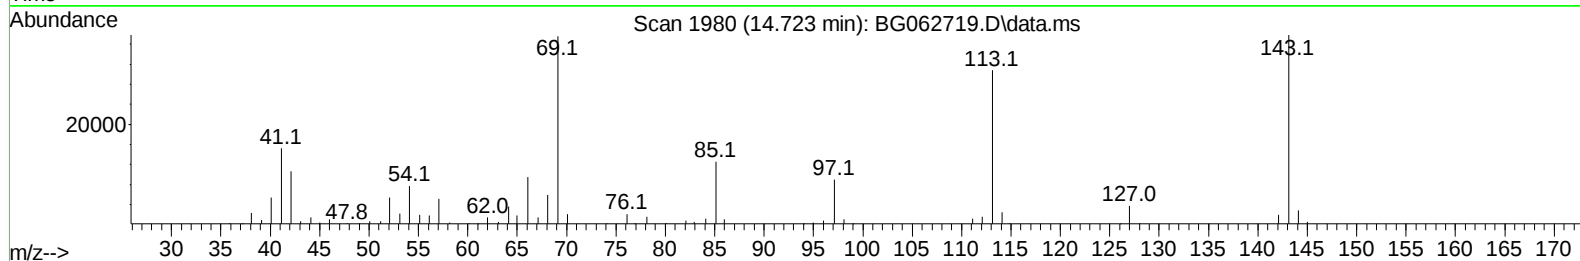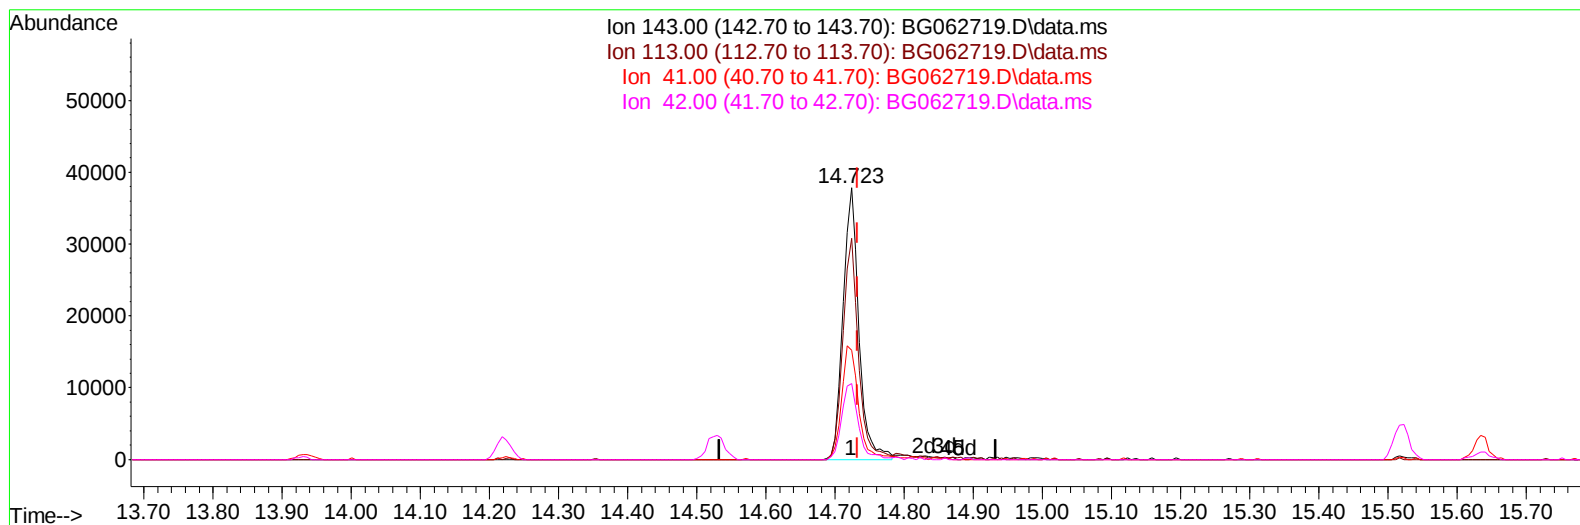

TIC: BG062719.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.723min (-0.009) 23.55 ng/ul m

response 59917

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.40	81.38
41.00	45.80	40.20
42.00	31.60	28.01

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062719.D
 Acq On : 11 Sep 2024 3:43
 Operator : JU/RC
 Sample : PB163242BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK242

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/12/2024
 Supervised By :mohammad ahmed 09/13/2024

Quant Time: Sep 11 04:37:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.902	152	56040	20.000	ng/ul	0.00
20) Naphthalene-d8	10.693	136	233134	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.529	164	194463	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.273	188	542095	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	650707	20.000	ng/ul	0.00
88) Perylene-d12	24.576	264	711784	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	7463	6.020	ng/uL	0.00
4) Pyridine-d5	3.766	84	108009	27.370	ng/ul	0.00
7) Phenol-d5	7.068	99	107471	21.870	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.232	67	67871	23.037	ng/ul	0.00
11) 2-Chlorophenol-d4	7.432	132	83267	23.263	ng/ul	0.00
15) 4-Methylphenol-d8	8.601	113	90643	22.135	ng/ul	0.00
21) Nitrobenzene-d5	9.054	128	41361	24.823	ng/ul	0.00
24) 2-Nitrophenol-d4	9.776	143	51391	28.201	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.317	165	91944	23.168	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	119805	21.962	ng/ul	0.00
46) Dimethylphthalate-d6	13.936	166	380112	25.383	ng/ul	0.00
49) Acenaphthylene-d8	14.224	160	403349	24.252	ng/ul	0.00
54) 4-Nitrophenol-d4	14.723	143	59917m	23.553	ng/ul	0.00
60) Fluorene-d10	15.522	176	341315	25.293	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	70555	22.627	ng/ul	0.00
73) Anthracene-d10	17.373	188	646811	25.282	ng/ul	0.00
81) Pyrene-d10	19.665	212	890588	24.322	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.371	264	918122	24.428	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062719.D
Acq On : 11 Sep 2024 3:43
Operator : JU/RC
Sample : PB163242BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK242

Manual IntegrationsAPPROVED

Quant Time: Sep 11 04:37:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/12/2024
Supervised By :mohammad ahmed 09/13/2024

