

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062722.D
 Acq On : 11 Sep 2024 5:44
 Operator : JU/RC
 Sample : P3877-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCVX3

Quant Time: Sep 11 06:21:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	66916	20.000	ng/ul	0.00
20) Naphthalene-d8	10.696	136	303242	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.527	164	255949	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.271	188	704142	20.000	ng/ul	0.00
79) Chrysene-d12	21.519	240	773878	20.000	ng/ul	0.00
88) Perylene-d12	24.580	264	849617	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	4955	3.347	ng/uL	0.00
4) Pyridine-d5	3.769	84	53261	11.303	ng/ul	0.00
7) Phenol-d5	7.065	99	79812	13.602	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.230	67	52638	14.963	ng/ul	0.00
11) 2-Chlorophenol-d4	7.435	132	74257	17.374	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	77679	15.886	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	34801	16.057	ng/ul	0.00
24) 2-Nitrophenol-d4	9.774	143	42733	18.029	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.314	165	86144	16.688	ng/ul	0.00
31) 4-Chloroaniline-d4	10.825	131	86482	12.188	ng/ul	0.00
46) Dimethylphthalate-d6	13.933	166	351273	17.822	ng/ul	0.00
49) Acenaphthylene-d8	14.221	160	368770	16.846	ng/ul	0.00
54) 4-Nitrophenol-d4	14.721	143	49766	14.863	ng/ul	-0.01
60) Fluorene-d10	15.520	176	313799	17.668	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.637	200	58448	14.430	ng/ul	0.00
73) Anthracene-d10	17.371	188	599555	18.042	ng/ul	0.00
81) Pyrene-d10	19.662	212	788791	18.113	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.368	264	814711	18.160	ng/ul	-0.01
Target Compounds						
71) Pentachlorophenol	16.924	266	93739	16.940	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062722.D
Acq On : 11 Sep 2024 5:44
Operator : JU/RC
Sample : P3877-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVX3


Quant Time: Sep 11 06:21:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

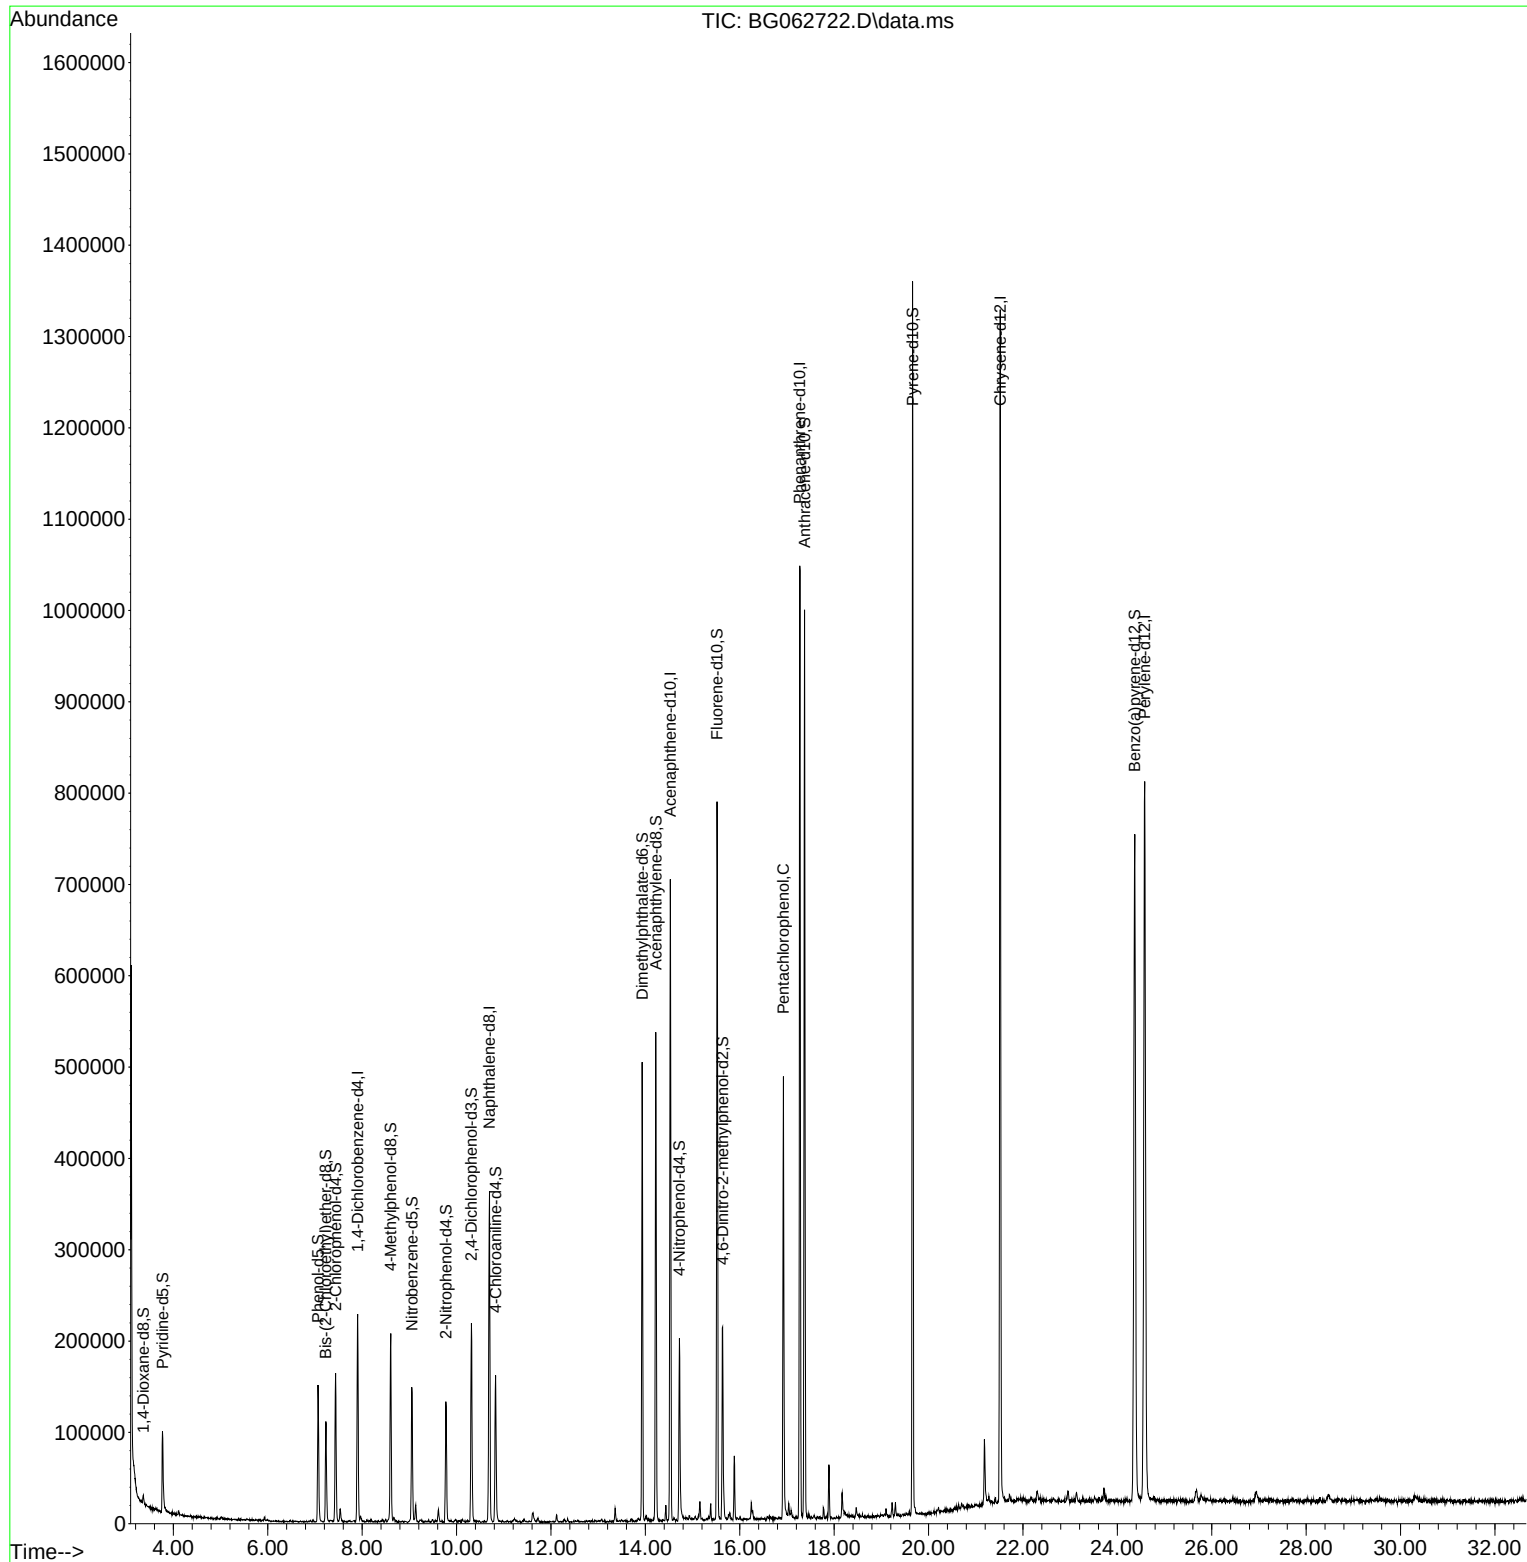

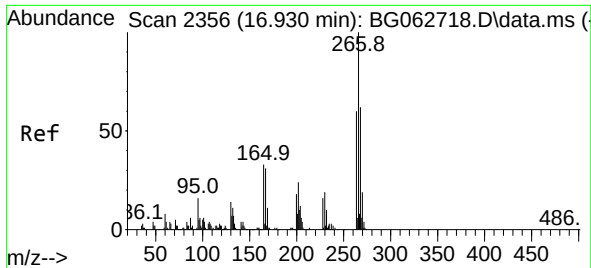

#71
 Pentachlorophenol
 Concen: 16.940 ng/ul
 RT: 16.924 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BG062722.D
 Acq: 11 Sep 2024 5:44

Instrument :
 BNA_G
 ClientSampleId :
 DCVX3

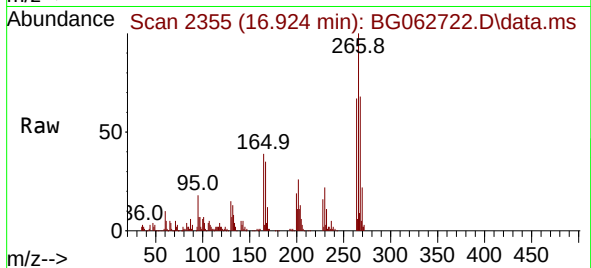

Tgt Ion	Ratio	Lower	Upper
266	100		
264	73.1	48.6	72.8#
268	68.3	49.5	74.3

