

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062697.D
 Acq On : 10 Sep 2024 9:54
 Operator : JU/RC
 Sample : PB163193BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK193

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	43	47	55	rVB4	15141	25000	1.00%	0.119%
2	3.769	112	116	135	rBV	176342	316774	12.66%	1.514%
3	4.093	168	171	172	rBV3	3638	3966	0.16%	0.019%
4	7.066	671	677	689	rVB	225144	377645	15.09%	1.804%
5	7.230	698	705	714	rBV	172247	288471	11.53%	1.378%
6	7.436	733	740	752	rBV	210281	360096	14.39%	1.721%
7	7.741	785	792	795	rBV5	1535	2776	0.11%	0.013%
8	7.906	813	820	832	rBV	212988	369649	14.77%	1.766%
9	8.605	932	939	950	rBV	273287	455614	18.21%	2.177%
10	9.057	1009	1016	1028	rBV	201464	363619	14.53%	1.737%
11	9.780	1130	1139	1150	rVB	162756	293309	11.72%	1.401%
12	10.315	1222	1230	1244	rBV	266546	475564	19.00%	2.272%
13	10.697	1286	1295	1304	rBV	306070	540595	21.60%	2.583%
14	10.826	1308	1317	1325	rBV	261829	467949	18.70%	2.236%
15	11.836	1486	1489	1494	rBV3	1644	2980	0.12%	0.014%
16	12.283	1560	1565	1567	rBV3	3332	4261	0.17%	0.020%
17	13.934	1837	1846	1854	rBV	623101	883203	35.29%	4.220%
18	14.222	1888	1895	1905	rBV	662804	1006500	40.22%	4.809%
19	14.527	1940	1947	1954	rBV	568529	884135	35.33%	4.224%
20	14.721	1973	1980	1993	rBV	262498	442276	17.67%	2.113%
21	15.091	2040	2043	2046	rBV2	2275	2708	0.11%	0.013%
22	15.520	2109	2116	2124	rBV	917310	1395918	55.78%	6.670%
23	15.638	2130	2136	2148	rBV	253934	390711	15.61%	1.867%
24	15.767	2155	2158	2164	rVB4	4063	6403	0.26%	0.031%
25	16.308	2247	2250	2253	rVB4	3251	3750	0.15%	0.018%
26	16.954	2357	2360	2364	rVB3	2569	2996	0.12%	0.014%
27	17.271	2407	2414	2425	rBV	851536	1269314	50.72%	6.065%
28	17.371	2425	2431	2442	rVV2	1153113	1719312	68.70%	8.215%
29	17.941	2525	2528	2532	rBV6	3138	4667	0.19%	0.022%
30	18.041	2543	2545	2551	rVB4	1650	2506	0.10%	0.012%
31	19.016	2707	2711	2714	rBV4	2161	3539	0.14%	0.017%
32	19.228	2742	2747	2753	rBV3	17814	26673	1.07%	0.127%
33	19.298	2756	2759	2764	rBV	12992	19425	0.78%	0.093%
34	19.498	2791	2793	2796	rBV4	2494	2859	0.11%	0.014%
35	19.663	2814	2821	2828	rBV	1667629	2321372	92.76%	11.092%
36	20.162	2904	2906	2909	rBV3	3472	4445	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062697.D
 Acq On : 10 Sep 2024 9:54
 Operator : JU/RC
 Sample : PB163193BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK193

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	20.462	2955	2957	2960	rBV3	2719	3007	0.12%	0.014%
38	20.603	2979	2981	2983	rBV3	2744	2707	0.11%	0.013%
39	20.738	3002	3004	3006	rBV3	3449	2777	0.11%	0.013%
40	21.055	3056	3058	3059	rBV	4244	2976	0.12%	0.014%
41	21.519	3130	3137	3150	rBV	1114726	1758847	70.28%	8.404%
42	22.295	3267	3269	3275	rVB6	8479	11045	0.44%	0.053%
43	22.959	3378	3382	3383	rBV4	7254	9781	0.39%	0.047%
44	23.634	3495	3497	3499	rBV3	6296	6142	0.25%	0.029%
45	24.369	3611	3622	3636	rBV2	968449	2502535	100.00%	11.957%
46	24.580	3646	3658	3675	rBV	671499	1839108	73.49%	8.787%
47	25.667	3838	3843	3844	rBV5	9857	15770	0.63%	0.075%
48	26.596	3999	4001	4002	rBV2	5260	3824	0.15%	0.018%
49	26.919	4054	4056	4057	rBV2	5862	3699	0.15%	0.018%
50	28.429	4311	4313	4314	rBV2	5067	4355	0.17%	0.021%
51	29.304	4460	4462	4463	rBV2	6401	3063	0.12%	0.015%
52	31.437	4823	4825	4828	rBV4	5317	6225	0.25%	0.030%
53	32.130	4941	4943	4947	rVB5	6469	6642	0.27%	0.032%
54	32.518	5007	5009	5012	rBV3	4939	5383	0.22%	0.026%


Sum of corrected areas: 20928866

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062697.D
Acq On : 10 Sep 2024 9:54
Operator : JU/RC
Sample : PB163193BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

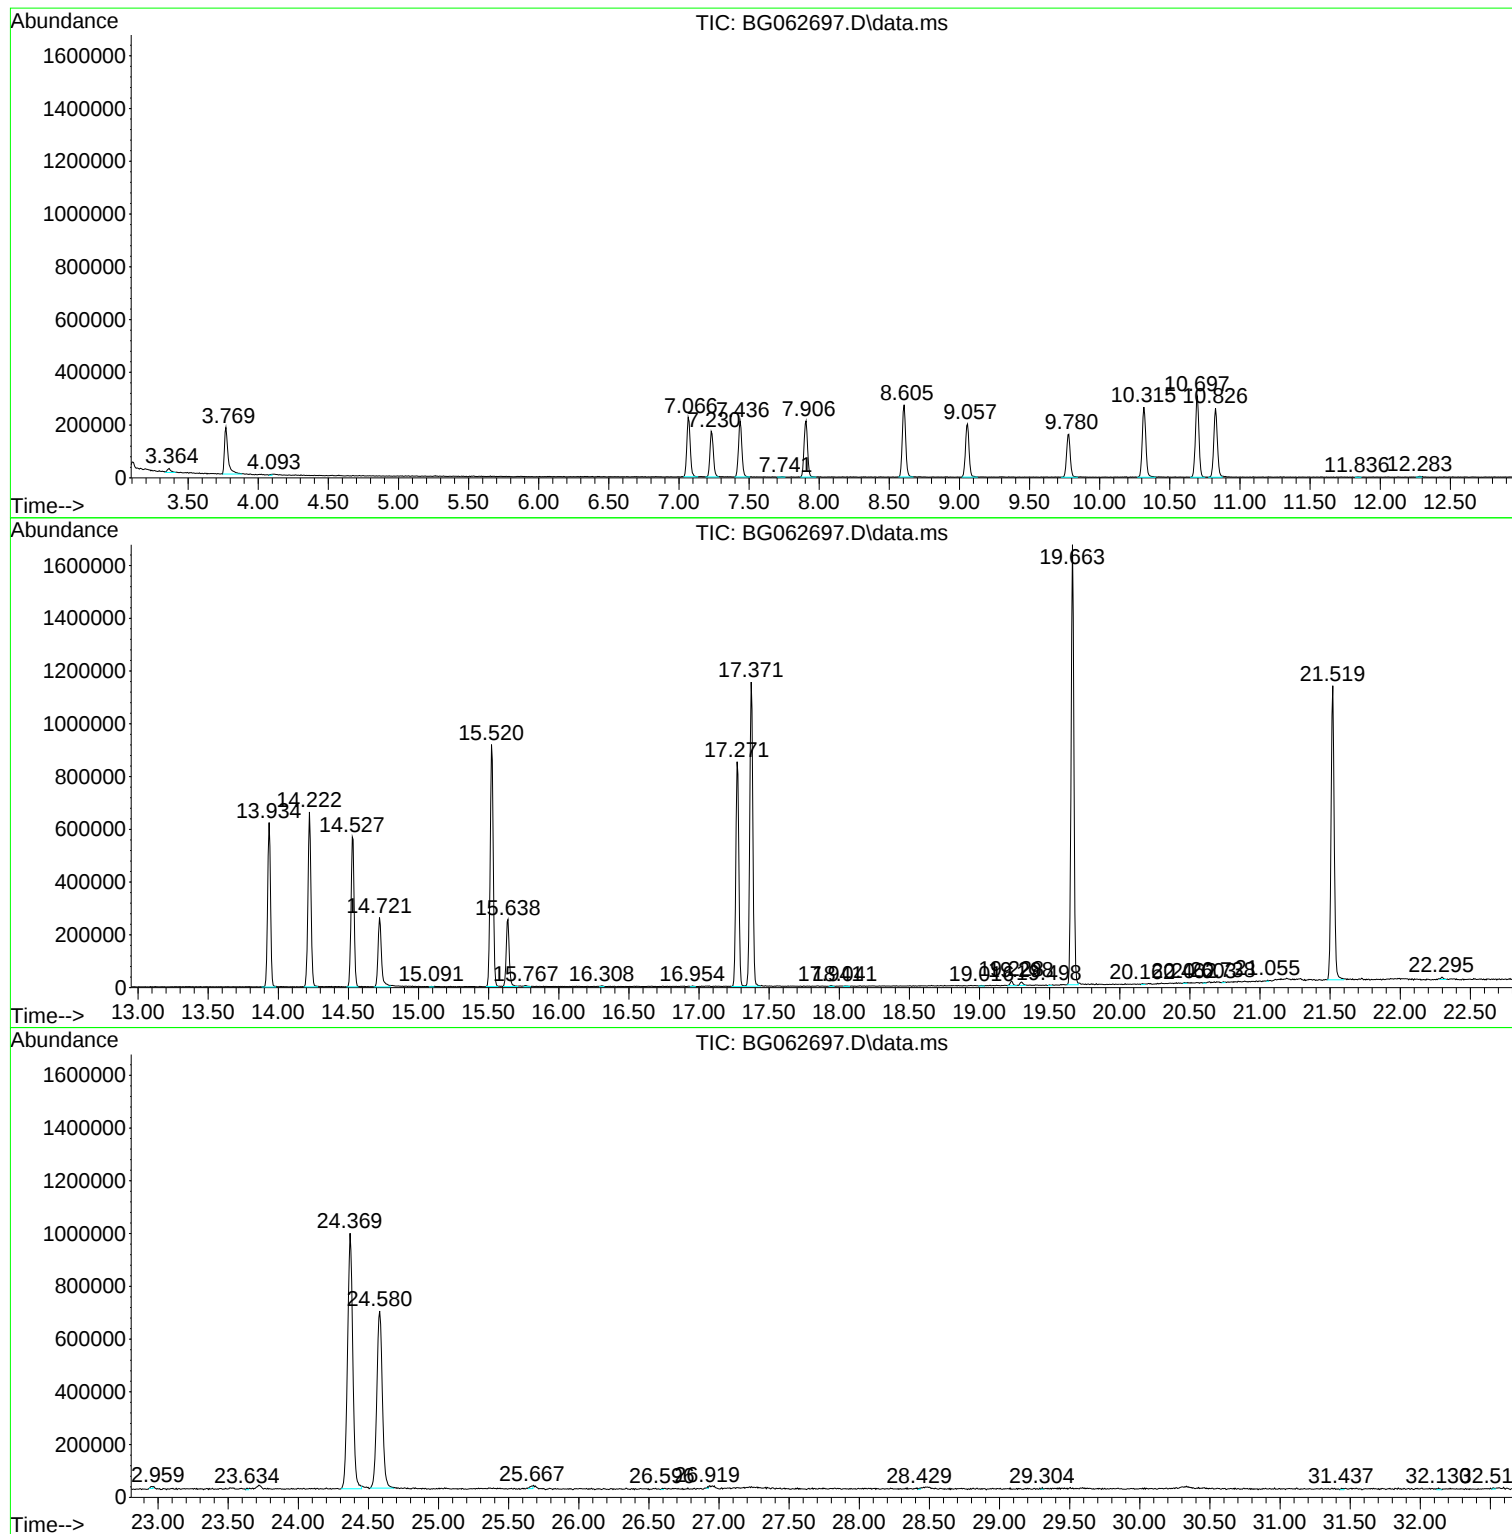

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062697.D
Acq On : 10 Sep 2024 9:54
Operator : JU/RC
Sample : PB163193BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062697.D
Acq On : 10 Sep 2024 9:54
Operator : JU/RC
Sample : PB163193BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc