

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062700.D
 Acq On : 10 Sep 2024 14:10
 Operator : JU/RC
 Sample : P3843-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHJM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.354	42	45	52	rVB3	15701	19324	0.69%	0.087%
2	3.765	111	115	122	rBV2	25547	46156	1.64%	0.208%
3	4.100	168	172	176	rVB4	3198	4526	0.16%	0.020%
4	4.899	305	308	312	rVB4	3456	3992	0.14%	0.018%
5	5.005	322	326	330	rBV5	2950	5400	0.19%	0.024%
6	6.162	518	523	528	rBV6	6133	10531	0.37%	0.047%
7	7.061	670	676	684	rVB	61969	102181	3.64%	0.460%
8	7.225	697	704	715	rBV	187006	309123	11.00%	1.392%
9	7.431	731	739	751	rBV	215800	350728	12.48%	1.579%
10	7.895	812	818	827	rVB	216069	369474	13.15%	1.663%
11	8.600	931	938	946	rBV	179928	296976	10.57%	1.337%
12	9.053	1008	1015	1024	rBV	232004	392859	13.98%	1.768%
13	9.775	1129	1138	1146	rBV	182457	326067	11.60%	1.468%
14	10.316	1222	1230	1242	rBV	292965	521337	18.55%	2.347%
15	10.692	1286	1294	1302	rBV	324917	572124	20.36%	2.575%
16	10.827	1310	1317	1327	rBV	195327	362750	12.91%	1.633%
17	12.278	1560	1564	1569	rBV4	4816	7765	0.28%	0.035%
18	12.513	1599	1604	1607	rVB2	4021	5071	0.18%	0.023%
19	13.935	1840	1846	1860	rVB	696438	982185	34.96%	4.421%
20	14.223	1888	1895	1904	rBV	728674	1146292	40.80%	5.160%
21	14.535	1940	1948	1954	rBV	612689	960194	34.17%	4.322%
22	14.728	1974	1981	1997	rBV5	79935	176336	6.28%	0.794%
23	14.952	2014	2019	2024	rBV5	3717	6399	0.23%	0.029%
24	15.527	2109	2117	2126	rBV	1056211	1596725	56.83%	7.188%
25	15.639	2129	2136	2148	rBV	313891	470599	16.75%	2.118%
26	15.763	2154	2157	2164	rVB5	3571	5634	0.20%	0.025%
27	17.061	2377	2378	2382	rVB2	2627	2891	0.10%	0.013%
28	17.278	2408	2415	2425	rBV	937622	1389059	49.44%	6.253%
29	17.378	2425	2432	2439	rBV	1346463	2020425	71.91%	9.095%
30	17.660	2476	2480	2483	rBV3	2154	2941	0.10%	0.013%
31	17.948	2526	2529	2534	rVB4	3292	4488	0.16%	0.020%
32	18.030	2539	2543	2546	rBV3	2316	2822	0.10%	0.013%
33	18.177	2562	2568	2572	rBV6	7668	15060	0.54%	0.068%
34	18.665	2647	2651	2653	rBV4	2739	3343	0.12%	0.015%
35	19.106	2721	2726	2727	rBV3	2968	3279	0.12%	0.015%
36	19.123	2727	2729	2733	rVB4	5174	4671	0.17%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062700.D
 Acq On : 10 Sep 2024 14:10
 Operator : JU/RC
 Sample : P3843-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHJM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	19.235	2742	2748	2754	rBV3	22053	32076	1.14%	0.144%
38	19.300	2754	2759	2765	rBV	18370	26686	0.95%	0.120%
39	19.599	2806	2810	2813	rBV4	5746	6576	0.23%	0.030%
40	19.670	2815	2822	2833	rBV	1921755	2783118	99.05%	12.528%
41	19.975	2872	2874	2877	rBV2	2582	3752	0.13%	0.017%
42	20.040	2880	2885	2886	rBV4	2310	3313	0.12%	0.015%
43	20.422	2948	2950	2951	rBV2	3972	3116	0.11%	0.014%
44	20.645	2986	2988	2990	rVB3	4979	3488	0.12%	0.016%
45	21.191	3078	3081	3082	rBV3	7736	8653	0.31%	0.039%
46	21.526	3131	3138	3147	rBV	1166850	1872573	66.64%	8.430%
47	21.826	3187	3189	3190	rBV2	4263	3098	0.11%	0.014%
48	22.302	3268	3270	3275	rVB4	12819	17765	0.63%	0.080%
49	22.960	3379	3382	3388	rVB5	17055	30819	1.10%	0.139%
50	23.730	3506	3513	3517	rBV7	21801	47229	1.68%	0.213%
51	24.382	3613	3624	3637	rBV	1089610	2809784	100.00%	12.649%
52	24.587	3648	3659	3676	rBV	691054	1967009	70.01%	8.855%
53	25.686	3841	3846	3858	rVB7	21944	59739	2.13%	0.269%
54	25.845	3871	3873	3875	rBV3	4575	4609	0.16%	0.021%
55	26.115	3917	3919	3923	rBV4	4703	4588	0.16%	0.021%
56	26.509	3984	3986	3991	rBV6	5263	8712	0.31%	0.039%
57	26.867	4045	4047	4049	rBV3	4233	3780	0.13%	0.017%
58	27.237	4108	4110	4113	rVB4	4841	4057	0.14%	0.018%
59	27.837	4210	4212	4218	rVV6	5953	6717	0.24%	0.030%
60	32.043	4926	4928	4929	rBV2	4385	3344	0.12%	0.015%




Sum of corrected areas: 22214328

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062700.D
Acq On : 10 Sep 2024 14:10
Operator : JU/RC
Sample : P3843-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

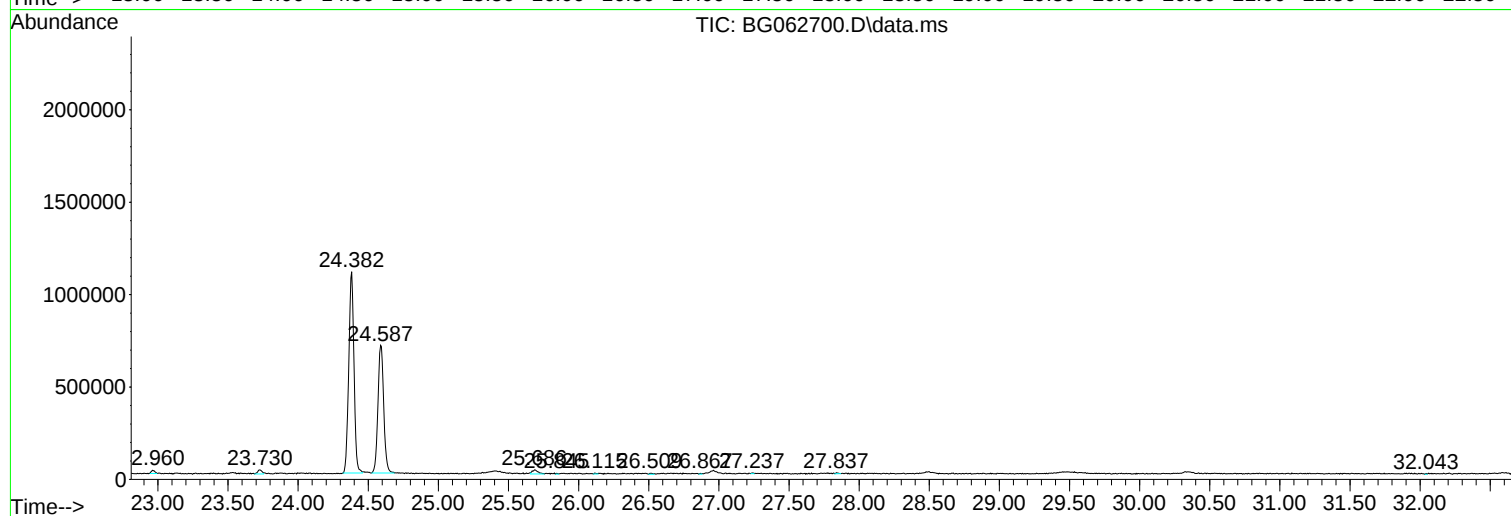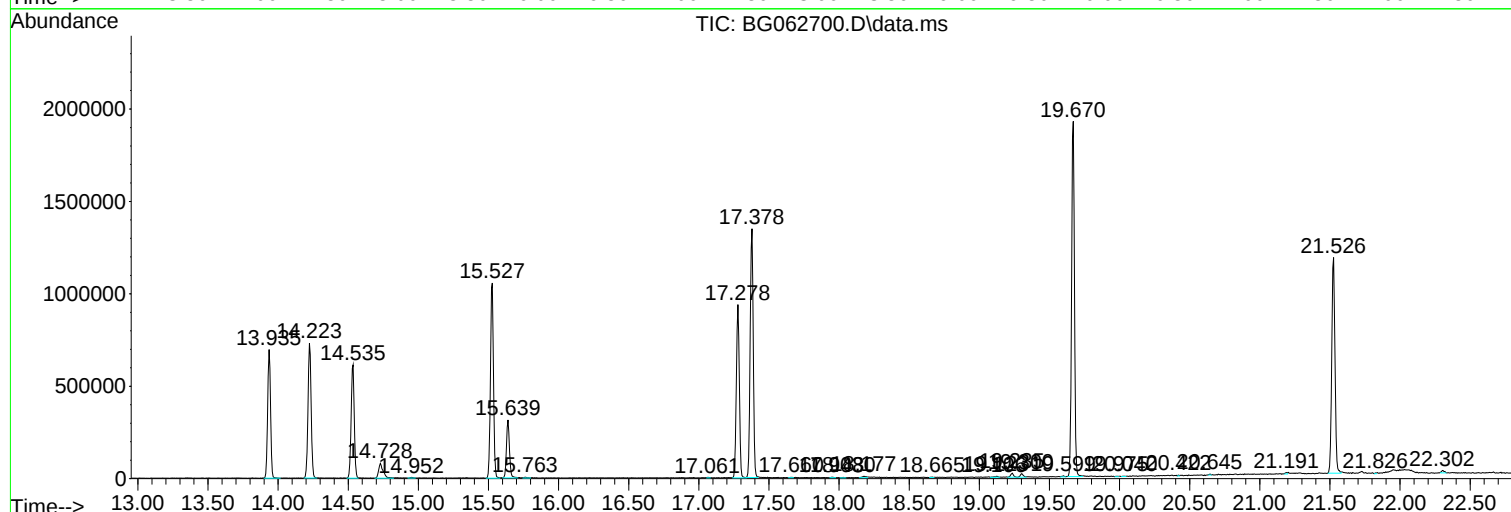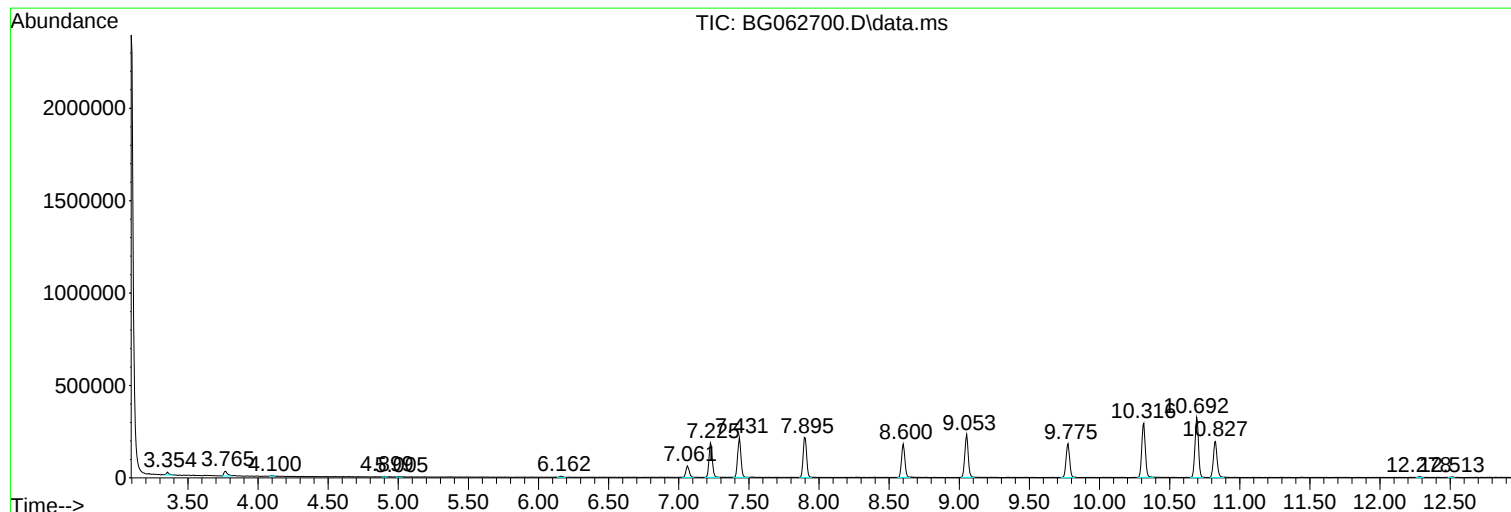

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062700.D
Acq On : 10 Sep 2024 14:10
Operator : JU/RC
Sample : P3843-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062700.D
Acq On : 10 Sep 2024 14:10
Operator : JU/RC
Sample : P3843-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc