

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062701.D
 Acq On : 10 Sep 2024 14:50
 Operator : JU/RC
 Sample : P3843-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHJM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	44	47	51	rVB2	10323	13632	0.50%	0.064%
2	3.769	113	116	124	rBV	53177	92811	3.41%	0.436%
3	4.034	159	161	164	rBV4	2026	2776	0.10%	0.013%
4	4.903	305	309	313	rBV5	3783	4852	0.18%	0.023%
5	5.015	325	328	332	rVB5	3071	4571	0.17%	0.021%
6	5.350	381	385	388	rBV4	2292	3696	0.14%	0.017%
7	6.166	522	524	530	rVB4	5484	8060	0.30%	0.038%
8	7.065	672	677	686	rBV	61574	105010	3.86%	0.493%
9	7.236	697	706	715	rBV	180846	310966	11.43%	1.459%
10	7.435	731	740	750	rBV	196392	349222	12.84%	1.639%
11	7.906	812	820	830	rBV	211623	360539	13.25%	1.692%
12	8.605	931	939	948	rBV2	179951	312141	11.48%	1.465%
13	8.669	948	950	955	rVB4	1922	3167	0.12%	0.015%
14	9.057	1009	1016	1026	rBV	220679	378760	13.92%	1.777%
15	9.780	1132	1139	1149	rBV	175024	312068	11.47%	1.465%
16	10.079	1188	1190	1197	rVB3	1932	3448	0.13%	0.016%
17	10.156	1197	1203	1206	rBV4	1831	2931	0.11%	0.014%
18	10.314	1223	1230	1241	rBV	276463	495094	18.20%	2.323%
19	10.696	1288	1295	1304	rBV	301169	532809	19.59%	2.500%
20	10.826	1310	1317	1326	rBV	269454	502170	18.46%	2.357%
21	12.283	1560	1565	1573	rVB7	4254	8488	0.31%	0.040%
22	13.940	1840	1847	1856	rBV	645340	932887	34.30%	4.378%
23	14.228	1888	1896	1903	rBV	694989	1094771	40.25%	5.138%
24	14.533	1941	1948	1957	rBV	581173	875440	32.18%	4.108%
25	14.727	1975	1981	1993	rBV2	51539	97430	3.58%	0.457%
26	15.526	2110	2117	2126	rBV	1035233	1535035	56.43%	7.204%
27	15.638	2130	2136	2143	rBV	305354	435058	15.99%	2.042%
28	15.767	2154	2158	2162	rVB3	4252	6957	0.26%	0.033%
29	17.036	2370	2374	2376	rBV3	2336	2933	0.11%	0.014%
30	17.277	2408	2415	2425	rBV	883061	1281067	47.10%	6.012%
31	17.377	2425	2432	2442	rVV	1309150	1968245	72.36%	9.237%
32	17.465	2444	2447	2453	rVB4	5317	8808	0.32%	0.041%
33	17.647	2472	2478	2481	rBV5	1797	3351	0.12%	0.016%
34	17.953	2526	2530	2533	rBV4	2638	3884	0.14%	0.018%
35	18.240	2576	2579	2585	rBV3	4025	5731	0.21%	0.027%
36	18.317	2587	2592	2595	rBV5	1537	2790	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062701.D
 Acq On : 10 Sep 2024 14:50
 Operator : JU/RC
 Sample : P3843-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHJM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	18.599	2635	2640	2641	rBV3	2867	3246	0.12%	0.015%
38	19.228	2743	2747	2754	rVB4	19572	27865	1.02%	0.131%
39	19.304	2754	2760	2763	rBV	17365	24279	0.89%	0.114%
40	19.668	2815	2822	2835	rBV	1881755	2692504	98.99%	12.636%
41	19.797	2842	2844	2847	rVB4	3180	2744	0.10%	0.013%
42	19.833	2847	2850	2852	rBV4	2766	3364	0.12%	0.016%
43	20.555	2971	2973	2975	rBV2	3479	3758	0.14%	0.018%
44	20.638	2985	2987	2989	rBV3	5817	5914	0.22%	0.028%
45	20.955	3039	3041	3045	rVB5	4790	4224	0.16%	0.020%
46	21.419	3117	3120	3125	rBV4	6519	9644	0.35%	0.045%
47	21.525	3131	3138	3149	rBV2	1028437	1699467	62.48%	7.975%
48	22.300	3268	3270	3277	rVB6	8557	11629	0.43%	0.055%
49	22.958	3378	3382	3387	rBV4	16853	29399	1.08%	0.138%
50	23.722	3506	3512	3520	rBV3	24137	56542	2.08%	0.265%
51	24.374	3612	3623	3639	rBV	1029626	2720085	100.00%	12.765%
52	24.586	3648	3659	3674	rBV	659700	1813407	66.67%	8.510%
53	25.685	3840	3846	3855	rVB6	24886	64327	2.36%	0.302%
54	26.037	3904	3906	3909	rBV4	4614	5735	0.21%	0.027%
55	26.948	4054	4061	4062	rBV5	23394	39385	1.45%	0.185%
56	27.230	4107	4109	4112	rBV4	5233	7252	0.27%	0.034%
57	28.417	4309	4311	4312	rBV2	4534	3321	0.12%	0.016%
58	29.968	4573	4575	4576	rVB2	6859	3388	0.12%	0.016%
59	31.830	4890	4892	4895	rBV4	4925	4136	0.15%	0.019%
60	32.289	4968	4970	4972	rBV3	4938	4559	0.17%	0.021%
61	32.553	5013	5015	5017	rBV3	5971	7051	0.26%	0.033%


Sum of corrected areas: 21308823

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062701.D
Acq On : 10 Sep 2024 14:50
Operator : JU/RC
Sample : P3843-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

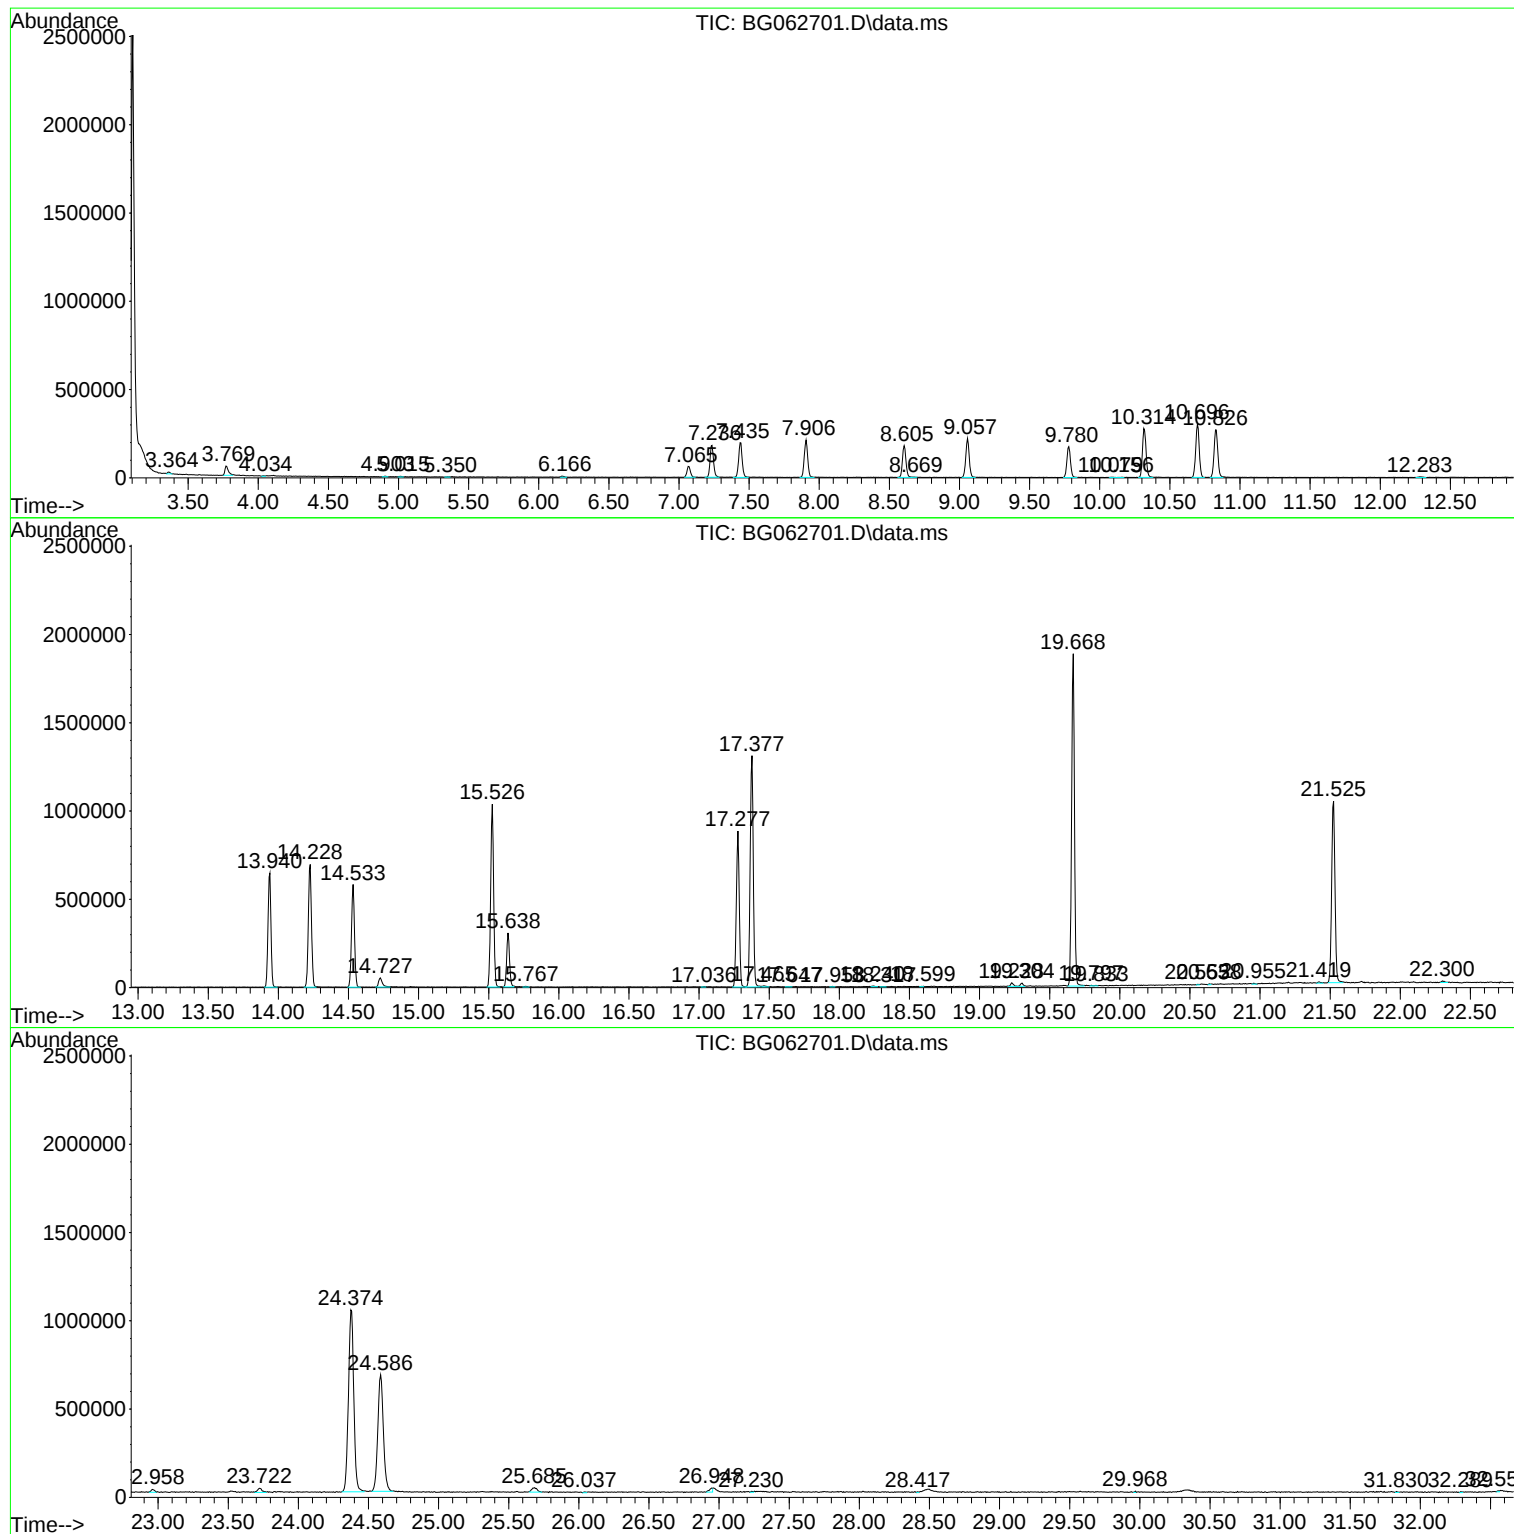

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062701.D
Acq On : 10 Sep 2024 14:50
Operator : JU/RC
Sample : P3843-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062701.D
Acq On : 10 Sep 2024 14:50
Operator : JU/RC
Sample : P3843-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc