

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062702.D
 Acq On : 10 Sep 2024 15:30
 Operator : JU/RC
 Sample : P3864-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH7N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.361	44	46	51	rVB2	11004	12677	0.44%	0.057%
2	3.778	115	117	123	rBV4	8659	11913	0.41%	0.053%
3	4.107	170	173	177	rVB4	3871	5777	0.20%	0.026%
4	4.677	268	270	273	rVB4	2410	2961	0.10%	0.013%
5	4.906	303	309	312	rBV5	3556	6757	0.24%	0.030%
6	5.576	421	423	429	rBV6	3513	5333	0.19%	0.024%
7	6.175	519	525	529	rBV4	7380	12085	0.42%	0.054%
8	7.068	669	677	685	rBV2	77496	144826	5.04%	0.648%
9	7.232	696	705	715	rBV	200723	355300	12.37%	1.589%
10	7.438	733	740	749	rBV	238666	414030	14.41%	1.852%
11	7.908	813	820	829	rBV	219749	384387	13.38%	1.719%
12	8.278	881	883	891	rVB5	2325	3596	0.13%	0.016%
13	8.607	931	939	949	rBV	211231	376044	13.09%	1.682%
14	9.060	1006	1016	1026	rBV	254756	450153	15.67%	2.014%
15	9.777	1128	1138	1150	rBV	204192	368066	12.81%	1.646%
16	10.317	1224	1230	1240	rBV	311052	569166	19.81%	2.546%
17	10.699	1287	1295	1304	rBV	325950	579043	20.15%	2.590%
18	10.828	1310	1317	1325	rVB3	21580	39490	1.37%	0.177%
19	12.291	1560	1566	1571	rBV6	4380	9991	0.35%	0.045%
20	13.936	1840	1846	1858	rBV	736724	1056388	36.77%	4.725%
21	14.224	1888	1895	1905	rBV	705628	1090256	37.95%	4.877%
22	14.530	1941	1947	1954	rBV	603129	931032	32.41%	4.165%
23	14.724	1975	1980	1994	rBV	82011	152517	5.31%	0.682%
24	14.947	2015	2018	2022	rVB5	3728	5554	0.19%	0.025%
25	15.529	2110	2117	2128	rBV	1109560	1707593	59.43%	7.638%
26	15.640	2130	2136	2147	rBV	351839	514394	17.90%	2.301%
27	15.764	2154	2157	2161	rVB5	4487	5473	0.19%	0.024%
28	16.751	2321	2325	2328	rBV3	1721	3183	0.11%	0.014%
29	17.280	2408	2415	2422	rBV	912706	1361630	47.39%	6.091%
30	17.374	2424	2431	2442	rBV	1361549	2117985	73.72%	9.474%
31	18.173	2563	2567	2573	rBV4	21063	34760	1.21%	0.155%
32	18.237	2575	2578	2583	rVB2	5011	7584	0.26%	0.034%
33	18.660	2646	2650	2652	rVV4	3363	4002	0.14%	0.018%
34	19.230	2742	2747	2752	rBV4	22832	34389	1.20%	0.154%
35	19.301	2754	2759	2765	rBV	20561	34573	1.20%	0.155%
36	19.448	2781	2784	2787	rBV4	7775	10175	0.35%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062702.D
Acq On : 10 Sep 2024 15:30
Operator : JU/RC
Sample : P3864-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH7N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Title : SVOA CALIBRATION

37	19.600	2807	2810	2812	rVB4	4221	5288	0.18%	0.024%
38	19.665	2814	2821	2829	rBV	2040477	2873087	100.00%	12.852%
39	20.576	2974	2976	2978	rVB2	4036	2956	0.10%	0.013%
40	20.693	2992	2996	2998	rBV4	4182	5536	0.19%	0.025%
41	20.869	3024	3026	3028	rVB3	5392	3155	0.11%	0.014%
42	21.151	3072	3074	3078	rBV5	5406	7781	0.27%	0.035%
43	21.522	3130	3137	3148	rBV2	1152683	1810648	63.02%	8.099%
44	22.891	3368	3370	3371	rBV2	4560	3129	0.11%	0.014%
45	22.961	3377	3382	3386	rBV8	12948	26079	0.91%	0.117%
46	23.231	3426	3428	3430	rBV3	4320	4020	0.14%	0.018%
47	23.513	3474	3476	3482	rVB7	6553	12282	0.43%	0.055%
48	23.725	3509	3512	3518	rVB6	15972	23604	0.82%	0.106%
49	24.377	3612	3623	3640	rBV	1108016	2850168	99.20%	12.749%
50	24.589	3648	3659	3674	rVB	687411	1878611	65.39%	8.403%
51	27.362	4129	4131	4132	rBV2	4459	3279	0.11%	0.015%
52	28.748	4365	4367	4369	rBV3	4827	4165	0.14%	0.019%
53	30.652	4689	4691	4698	rBV7	4923	8496	0.30%	0.038%
54	31.821	4889	4890	4892	rBV2	6064	3471	0.12%	0.016%
55	32.021	4922	4924	4925	rVB2	5487	2931	0.10%	0.013%
56	32.221	4956	4958	4959	rBV2	4190	4029	0.14%	0.018%




Sum of corrected areas: 22355798

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062702.D
Acq On : 10 Sep 2024 15:30
Operator : JU/RC
Sample : P3864-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH7N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

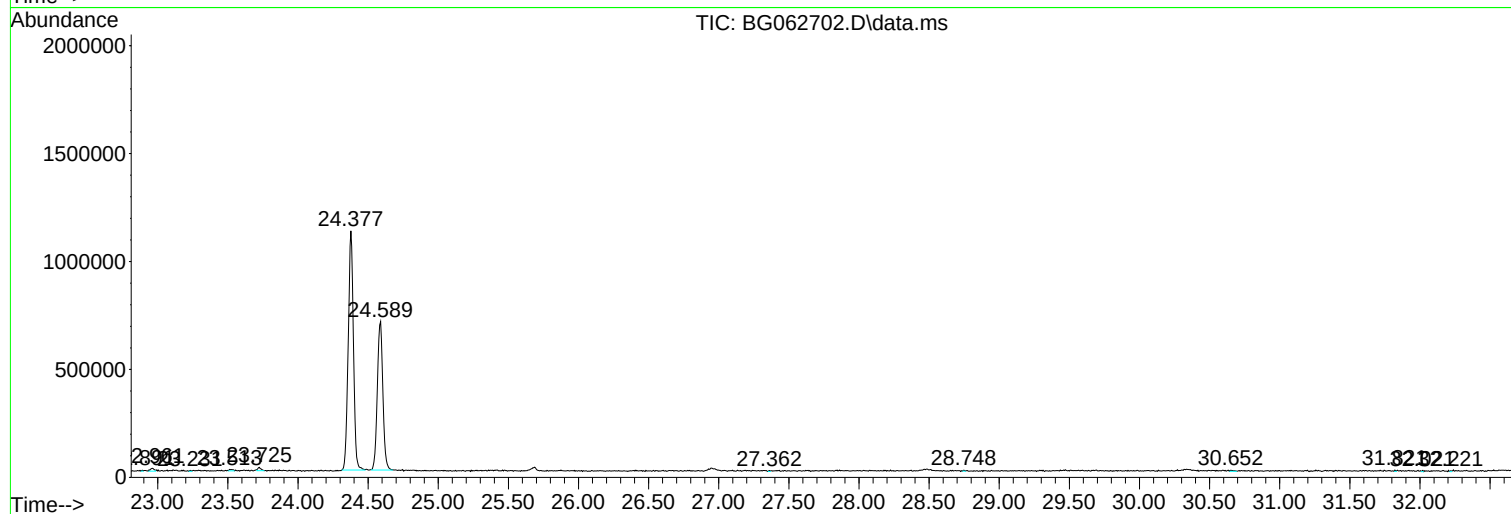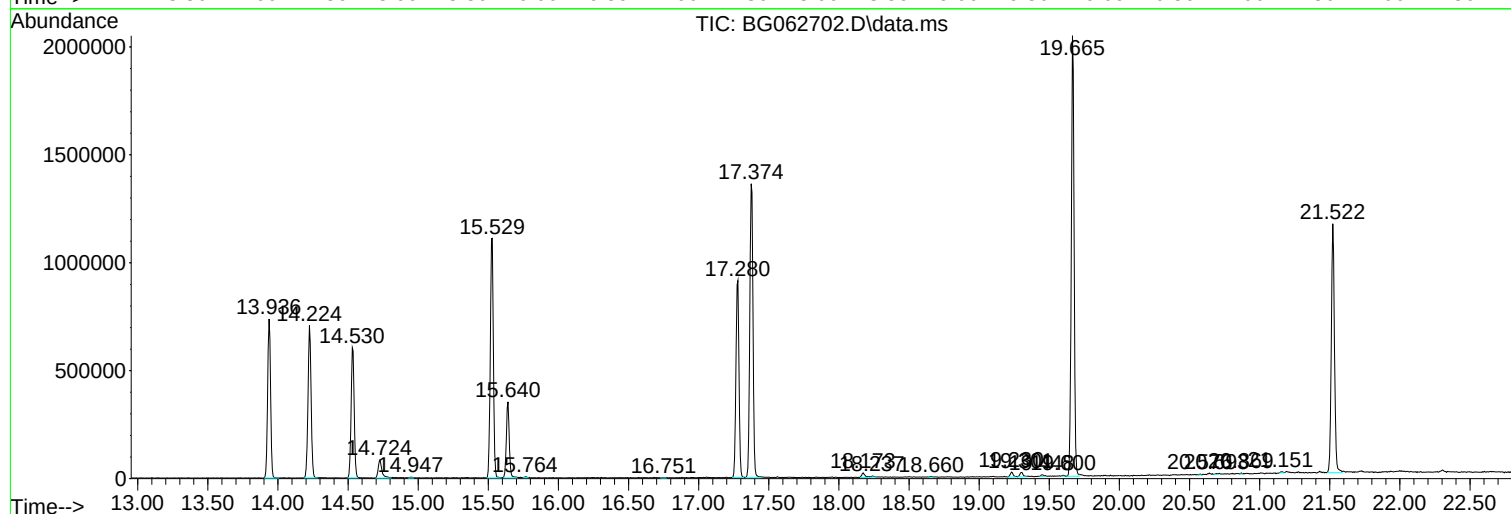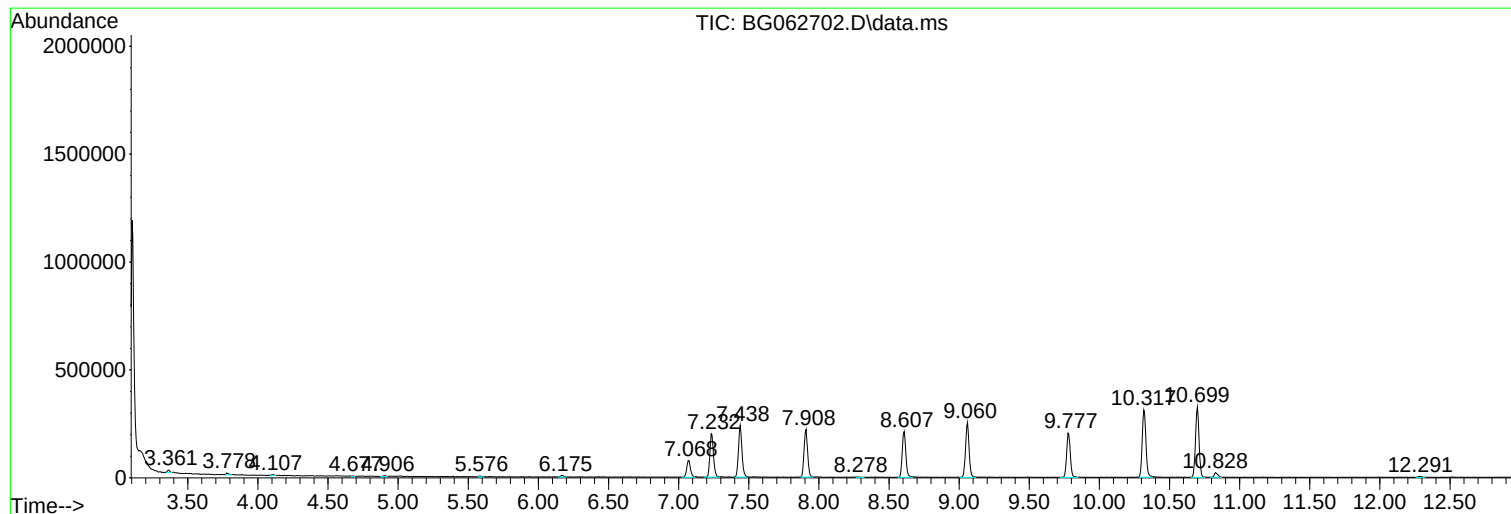

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062702.D
Acq On : 10 Sep 2024 15:30
Operator : JU/RC
Sample : P3864-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH7N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062702.D
Acq On : 10 Sep 2024 15:30
Operator : JU/RC
Sample : P3864-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH7N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc