

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062704.D
 Acq On : 10 Sep 2024 16:51
 Operator : JU/RC
 Sample : PB163196BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK196

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.360	43	46	56	rVB4	16994	32959	1.12%	0.129%
2	3.559	79	80	85	rBV4	3219	2948	0.10%	0.012%
3	3.765	111	115	126	rVV	207537	347797	11.86%	1.359%
4	4.106	169	173	176	rBV3	4648	6016	0.21%	0.024%
5	7.067	669	677	687	rBV	255847	439828	15.00%	1.719%
6	7.232	697	705	716	rVB	197489	327214	11.16%	1.279%
7	7.437	733	740	751	rBV	242455	409149	13.95%	1.599%
8	7.901	812	819	830	rBV	256938	439937	15.00%	1.719%
9	8.606	931	939	950	rBV	313960	532462	18.16%	2.081%
10	9.053	1007	1015	1026	rBV	234027	418107	14.26%	1.634%
11	9.776	1131	1138	1150	rBV	195202	346985	11.83%	1.356%
12	10.316	1222	1230	1242	rBV	315466	559311	19.08%	2.186%
13	10.698	1287	1295	1302	rBV	377561	672191	22.93%	2.627%
14	10.827	1309	1317	1331	rBV	312445	561233	19.14%	2.194%
15	12.284	1558	1565	1568	rBV4	5021	9074	0.31%	0.035%
16	12.884	1664	1667	1670	rBV3	2175	3020	0.10%	0.012%
17	13.935	1840	1846	1854	rBV	745577	1055044	35.98%	4.124%
18	14.223	1886	1895	1903	rBV	773180	1209803	41.26%	4.729%
19	14.529	1938	1947	1954	rBV	728622	1136342	38.76%	4.441%
20	14.723	1974	1980	1993	rBV	316619	533342	18.19%	2.085%
21	15.522	2109	2116	2125	rBV	1138091	1672035	57.03%	6.535%
22	15.639	2129	2136	2144	rBV	328651	497287	16.96%	1.944%
23	15.763	2153	2157	2161	rVB5	5538	8469	0.29%	0.033%
24	17.273	2407	2414	2424	rBV	1112208	1653907	56.41%	6.464%
25	17.373	2424	2431	2443	rVV	1411246	2089608	71.27%	8.167%
26	17.943	2524	2528	2532	rVB4	3237	4257	0.15%	0.017%
27	19.229	2741	2747	2753	rBV3	18881	30776	1.05%	0.120%
28	19.300	2755	2759	2766	rVV2	18471	26469	0.90%	0.103%
29	19.594	2805	2809	2814	rBV5	3877	6569	0.22%	0.026%
30	19.664	2814	2821	2834	rBV	1995230	2829893	96.52%	11.061%
31	20.093	2891	2894	2898	rBV5	2262	3439	0.12%	0.013%
32	20.404	2942	2947	2949	rBV4	3914	5653	0.19%	0.022%
33	20.581	2975	2977	2978	rBV2	3870	3403	0.12%	0.013%
34	20.645	2985	2988	2993	rBV4	6148	6883	0.23%	0.027%
35	20.698	2995	2997	3001	rBV4	2960	3245	0.11%	0.013%
36	21.021	3049	3052	3053	rBV3	3681	4355	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062704.D
 Acq On : 10 Sep 2024 16:51
 Operator : JU/RC
 Sample : PB163196BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK196

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	21.286	3093	3097	3098	rBV3	3607	4299	0.15%	0.017%
38	21.521	3130	3137	3148	rBV	1424352	2199263	75.01%	8.596%
39	22.572	3314	3316	3320	rBV5	4092	3931	0.13%	0.015%
40	22.960	3378	3382	3388	rVB7	17037	29825	1.02%	0.117%
41	23.524	3474	3478	3481	rBV5	5621	10452	0.36%	0.041%
42	23.718	3507	3511	3516	rVB6	16790	32934	1.12%	0.129%
43	24.370	3611	3622	3640	rBV2	1079915	2932053	100.00%	11.460%
44	24.582	3647	3658	3673	rBV	850521	2307263	78.69%	9.018%
45	25.675	3839	3844	3854	rVB6	21672	59605	2.03%	0.233%
46	25.998	3897	3899	3901	rBV3	4148	3940	0.13%	0.015%
47	26.809	4035	4037	4038	rBV2	5701	4263	0.15%	0.017%
48	26.950	4054	4061	4072	rVB8	19040	61185	2.09%	0.239%
49	27.602	4169	4172	4174	rBV4	5426	4610	0.16%	0.018%
50	28.348	4297	4299	4303	rBV5	4402	4393	0.15%	0.017%
51	28.471	4315	4320	4322	rBV6	10783	19725	0.67%	0.077%
52	29.188	4440	4442	4446	rBV5	4287	3924	0.13%	0.015%
53	29.541	4501	4502	4507	rBV4	6190	4945	0.17%	0.019%
54	29.623	4514	4516	4517	rVB2	4941	3005	0.10%	0.012%
55	30.698	4697	4699	4701	rBV3	4734	3126	0.11%	0.012%
56	32.473	4999	5001	5003	rBV3	4281	3479	0.12%	0.014%




Sum of corrected areas: 25585230

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062704.D
Acq On : 10 Sep 2024 16:51
Operator : JU/RC
Sample : PB163196BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK196

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

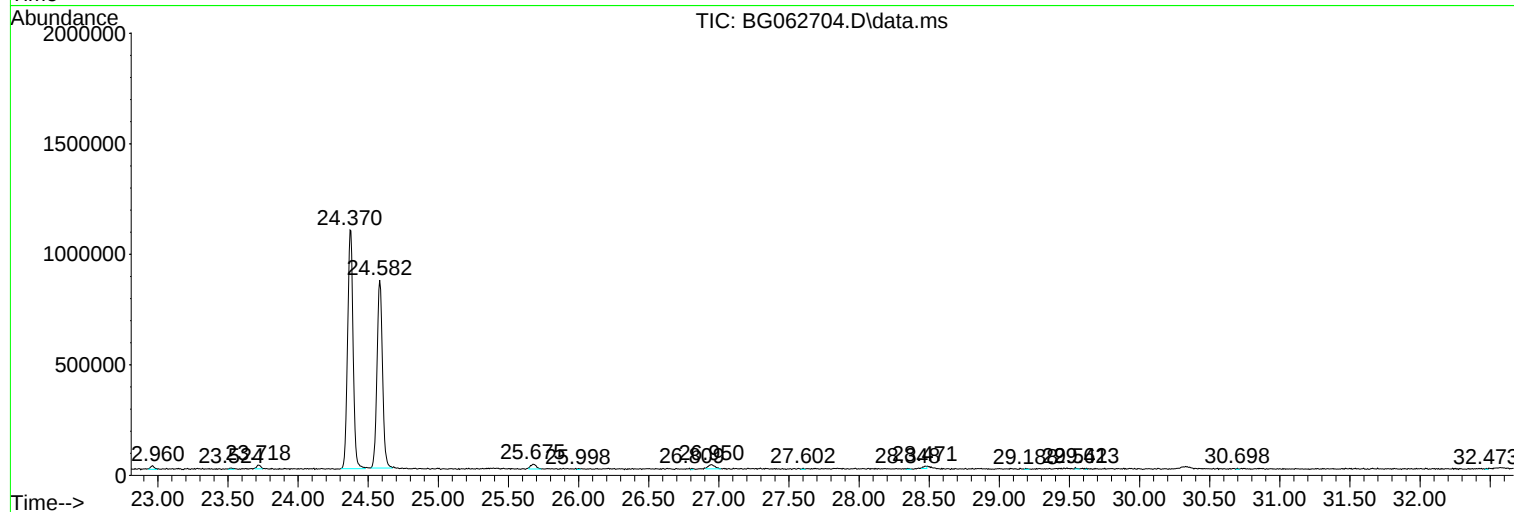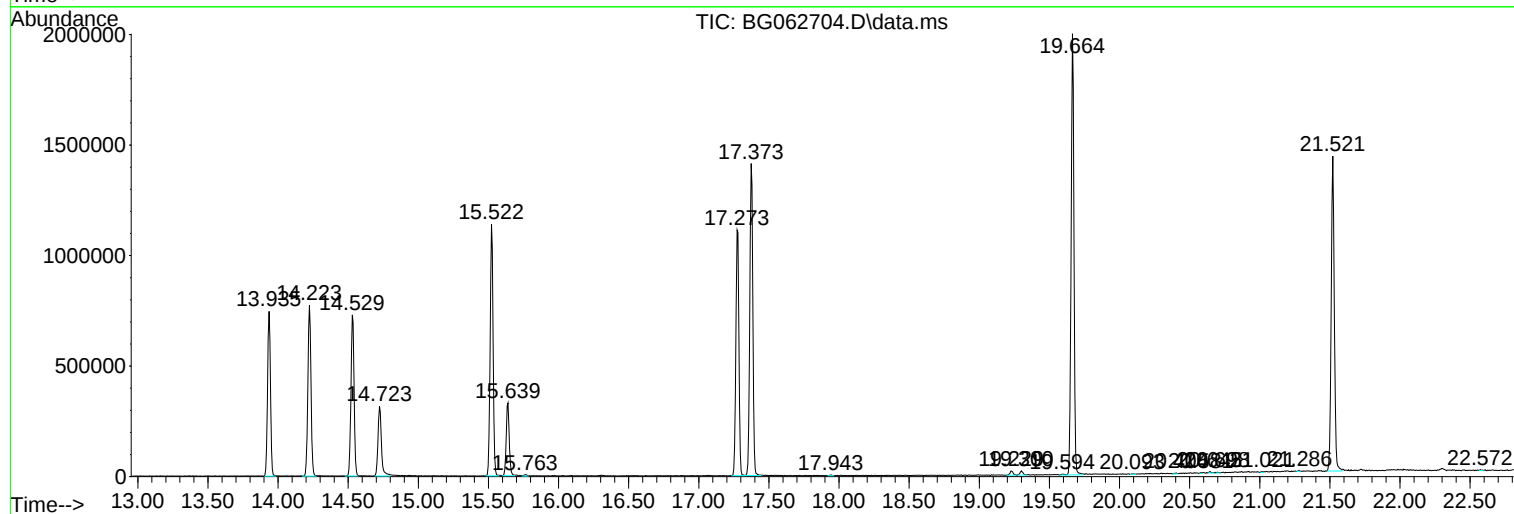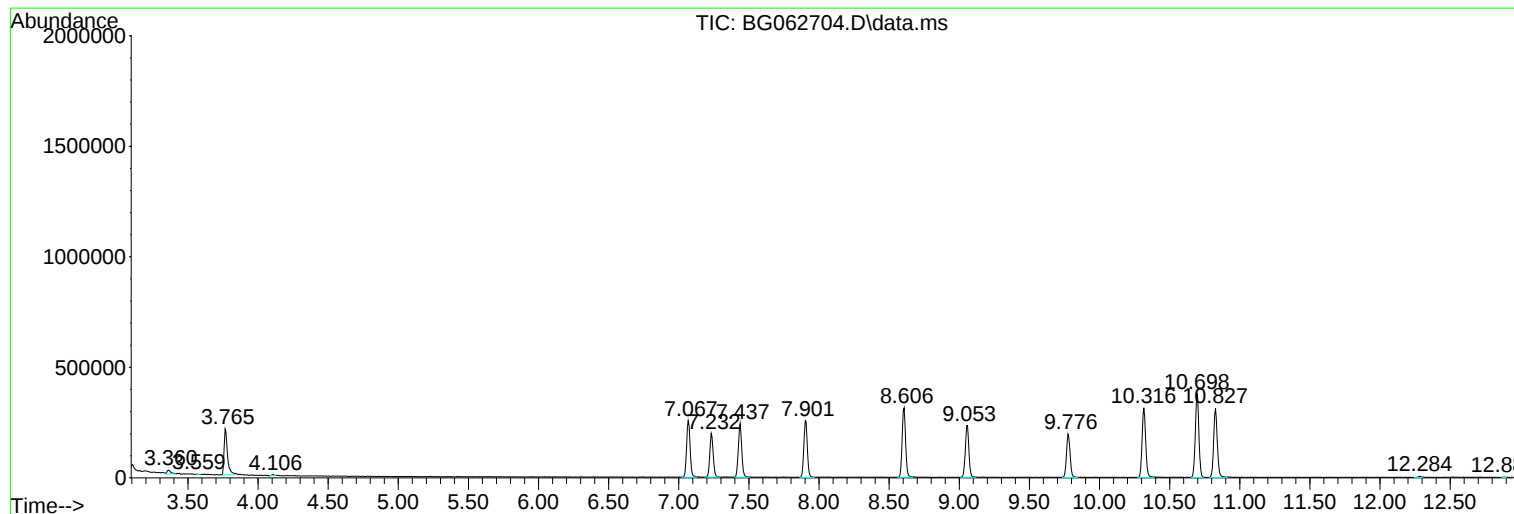

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062704.D
Acq On : 10 Sep 2024 16:51
Operator : JU/RC
Sample : PB163196BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK196

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062704.D
Acq On : 10 Sep 2024 16:51
Operator : JU/RC
Sample : PB163196BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK196

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc