

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062705.D
 Acq On : 10 Sep 2024 17:33
 Operator : JU/RC
 Sample : PB163198BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	50	rVB3	12005	13759	0.52%	0.063%
2	3.768	112	116	134	rBV	180743	330460	12.61%	1.513%
3	7.070	671	678	693	rBV	222957	403208	15.38%	1.846%
4	7.235	699	706	717	rVB	174757	303111	11.56%	1.388%
5	7.435	734	740	751	rBV	212664	381561	14.56%	1.747%
6	7.905	811	820	828	rBV	208770	362470	13.83%	1.660%
7	8.604	931	939	955	rBV	292188	494519	18.87%	2.264%
8	9.056	1009	1016	1026	rBV	212907	380233	14.51%	1.741%
9	9.779	1129	1139	1150	rBV	177907	314201	11.99%	1.439%
10	10.314	1223	1230	1241	rBV	271694	497129	18.96%	2.276%
11	10.696	1286	1295	1304	rBV	302252	536655	20.47%	2.457%
12	10.825	1310	1317	1330	rBV	270376	503712	19.22%	2.307%
13	11.630	1450	1454	1457	rBV3	1849	2647	0.10%	0.012%
14	12.282	1560	1565	1566	rBV3	4595	4483	0.17%	0.021%
15	13.845	1827	1831	1836	rBV4	1362	2789	0.11%	0.013%
16	13.933	1839	1846	1857	rVB	644322	932396	35.57%	4.270%
17	14.221	1887	1895	1903	rBV2	672035	1069157	40.79%	4.896%
18	14.532	1939	1948	1958	rVB	561418	884893	33.76%	4.052%
19	14.726	1973	1981	1991	rBV	269778	460717	17.58%	2.110%
20	14.861	2002	2004	2009	rVB4	2572	3692	0.14%	0.017%
21	15.525	2110	2117	2130	rVB	976743	1483499	56.59%	6.793%
22	15.637	2130	2136	2144	rBV	296966	428510	16.35%	1.962%
23	15.760	2155	2157	2160	rVB3	2244	2670	0.10%	0.012%
24	16.089	2208	2213	2217	rBV4	2226	4005	0.15%	0.018%
25	16.307	2247	2250	2255	rBV4	3772	6987	0.27%	0.032%
26	17.276	2408	2415	2425	rBV	846693	1284520	49.00%	5.882%
27	17.370	2425	2431	2440	rVV	1208363	1833303	69.94%	8.395%
28	17.429	2440	2441	2447	rVB5	3760	4930	0.19%	0.023%
29	17.840	2507	2511	2514	rVB2	2300	3301	0.13%	0.015%
30	17.946	2525	2529	2531	rBV5	2368	2746	0.10%	0.013%
31	19.227	2742	2747	2751	rBV4	17892	26819	1.02%	0.123%
32	19.303	2754	2760	2767	rBV	15891	25618	0.98%	0.117%
33	19.397	2772	2776	2779	rBV4	2302	4191	0.16%	0.019%
34	19.544	2800	2801	2805	rBV3	2342	3348	0.13%	0.015%
35	19.662	2814	2821	2836	rBV	1767764	2520439	96.15%	11.542%
36	20.631	2984	2986	2990	rBV5	5476	6795	0.26%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062705.D
 Acq On : 10 Sep 2024 17:33
 Operator : JU/RC
 Sample : PB163198BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	20.778	3009	3011	3013	rBV2	3369	3152	0.12%	0.014%
38	21.031	3052	3054	3057	rVB4	3766	3266	0.12%	0.015%
39	21.172	3076	3078	3079	rBV2	4639	3491	0.13%	0.016%
40	21.518	3130	3137	3145	rBV2	1079543	1707397	65.13%	7.818%
41	21.718	3168	3171	3175	rBV5	7695	12753	0.49%	0.058%
42	21.900	3200	3202	3203	rBV2	4348	2684	0.10%	0.012%
43	22.194	3250	3252	3254	rBV3	4686	4121	0.16%	0.019%
44	22.958	3379	3382	3387	rVB7	12185	18035	0.69%	0.083%
45	23.257	3431	3433	3434	rBV2	4963	4606	0.18%	0.021%
46	23.716	3509	3511	3519	rVB7	18818	32957	1.26%	0.151%
47	24.374	3611	3623	3637	rBV2	988718	2621335	100.00%	12.004%
48	24.579	3647	3658	3673	rBV	650075	1798406	68.61%	8.235%
49	24.908	3712	3714	3718	rBV5	4135	4540	0.17%	0.021%
50	24.997	3727	3729	3730	rBV2	5493	3423	0.13%	0.016%
51	25.055	3737	3739	3741	rBV3	5413	4651	0.18%	0.021%
52	25.678	3839	3845	3853	rVB9	20456	49367	1.88%	0.226%
53	26.142	3922	3924	3928	rVB5	5569	5471	0.21%	0.025%
54	26.847	4042	4044	4046	rBV2	3938	2908	0.11%	0.013%
55	26.871	4046	4048	4050	rBV3	4106	3762	0.14%	0.017%
56	27.035	4074	4076	4080	rBV5	4724	5902	0.23%	0.027%
57	27.975	4234	4236	4241	rBV5	4067	4836	0.18%	0.022%
58	30.490	4662	4664	4666	rBV2	4469	2839	0.11%	0.013%
59	31.213	4785	4787	4790	rBV4	5720	6329	0.24%	0.029%
60	31.812	4887	4889	4892	rBV4	4119	3820	0.15%	0.017%
61	31.988	4918	4919	4921	rBV2	4367	4463	0.17%	0.020%




Sum of corrected areas: 21837987

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062705.D
Acq On : 10 Sep 2024 17:33
Operator : JU/RC
Sample : PB163198BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

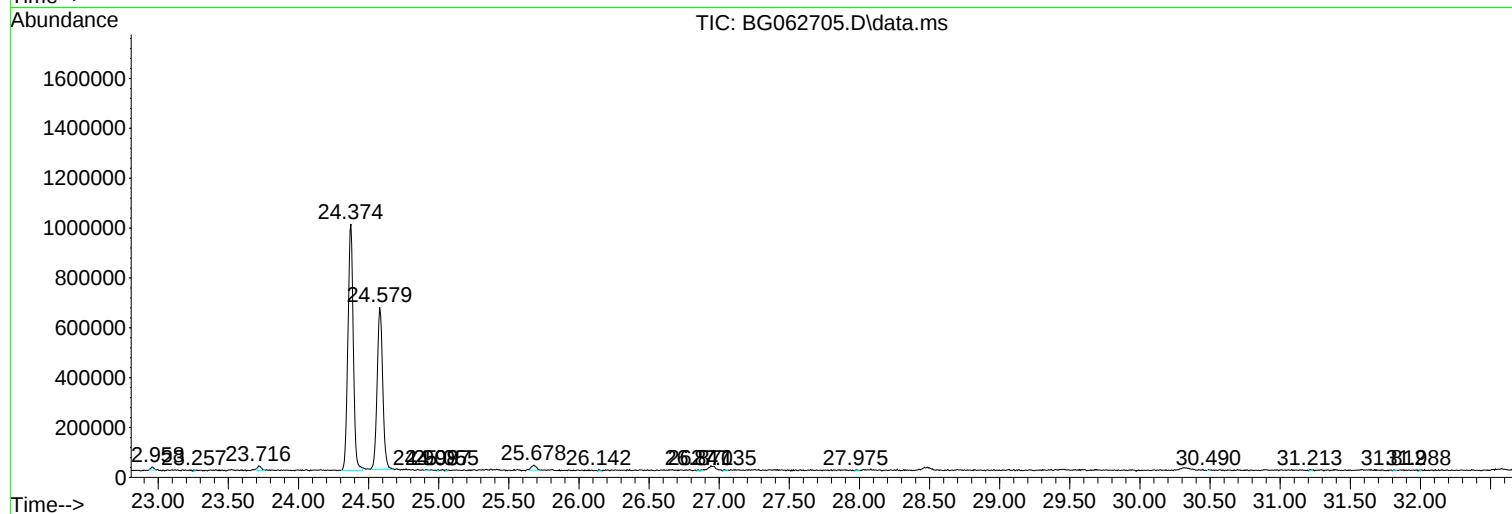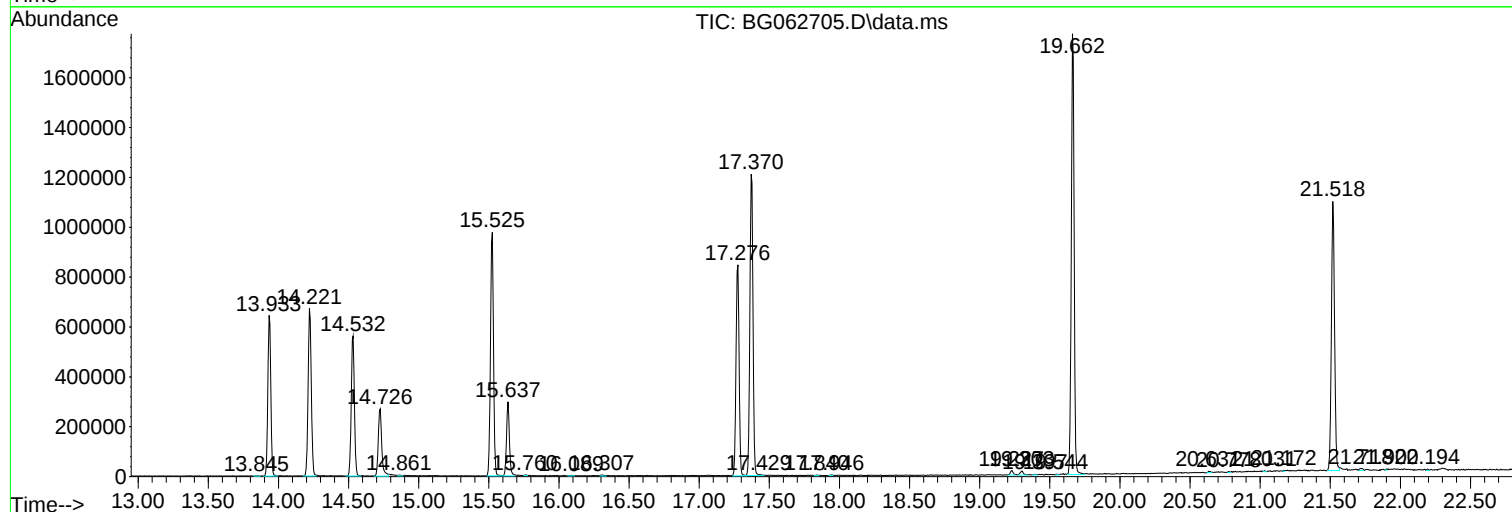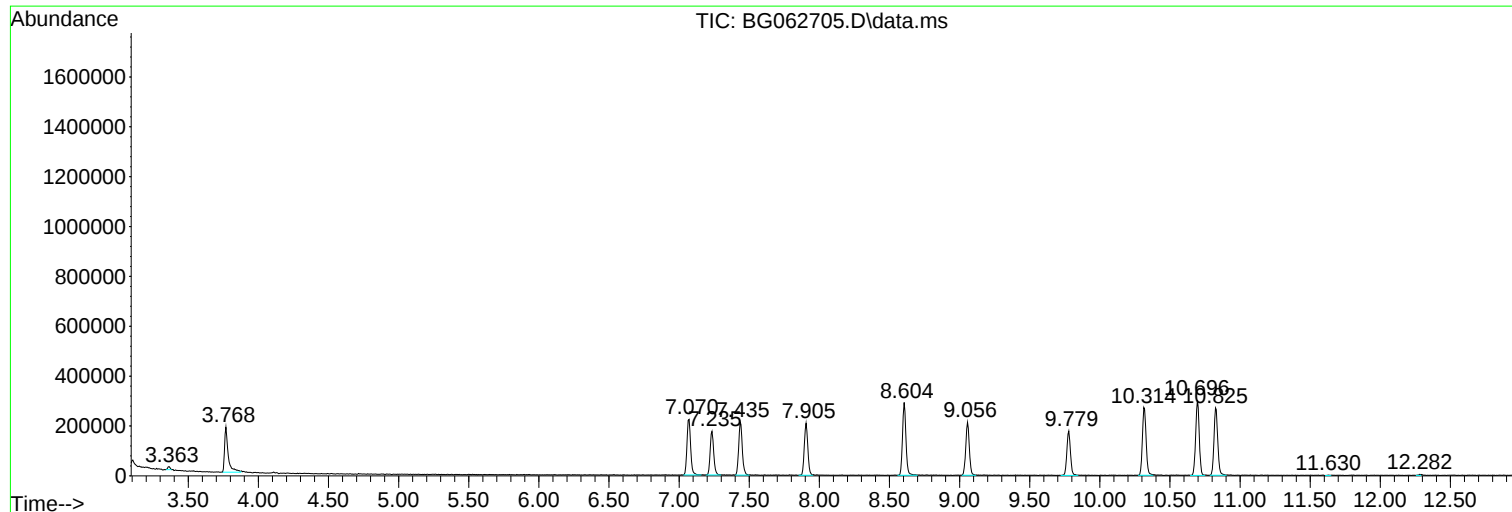

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062705.D
Acq On : 10 Sep 2024 17:33
Operator : JU/RC
Sample : PB163198BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062705.D
Acq On : 10 Sep 2024 17:33
Operator : JU/RC
Sample : PB163198BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
