

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062707.D
 Acq On : 10 Sep 2024 18:55
 Operator : JU/RC
 Sample : P3843-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHJM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.365	44	47	52	rVB2	14655	17742	0.63%	0.080%
2	3.629	88	92	100	rVB	19910	28219	1.01%	0.127%
3	3.770	113	116	127	rBV	41311	78391	2.79%	0.353%
4	3.929	140	143	148	rVB5	3111	6074	0.22%	0.027%
5	4.011	155	157	161	rVB4	3073	3362	0.12%	0.015%
6	4.111	169	174	178	rVB5	3757	6255	0.22%	0.028%
7	5.010	325	327	331	rVB4	2303	2810	0.10%	0.013%
8	6.167	519	524	532	rVB7	6001	11559	0.41%	0.052%
9	7.066	671	677	689	rBV	77433	136696	4.87%	0.615%
10	7.231	699	705	717	rVB	193495	325758	11.61%	1.466%
11	7.436	733	740	754	rBV	215650	377285	13.45%	1.698%
12	7.906	813	820	829	rBV	229507	402526	14.35%	1.812%
13	8.605	931	939	948	rBV	218006	380203	13.56%	1.711%
14	9.058	1008	1016	1029	rBV	225221	411026	14.65%	1.850%
15	9.775	1131	1138	1149	rBV	181136	330945	11.80%	1.490%
16	10.315	1223	1230	1242	rBV	290038	525328	18.73%	2.364%
17	10.691	1287	1294	1304	rBV	324210	589868	21.03%	2.655%
18	10.826	1310	1317	1327	rBV2	242069	449579	16.03%	2.023%
19	12.284	1557	1565	1571	rBV4	4350	8533	0.30%	0.038%
20	13.935	1839	1846	1853	rBV	655616	932550	33.25%	4.197%
21	14.222	1888	1895	1909	rVB2	725110	1118860	39.89%	5.036%
22	14.528	1940	1947	1956	rBV	612405	953222	33.99%	4.290%
23	14.722	1975	1980	1991	rBV3	57197	112588	4.01%	0.507%
24	14.945	2013	2018	2021	rBV3	3250	4906	0.17%	0.022%
25	15.521	2110	2116	2124	rBV	1028524	1557465	55.53%	7.010%
26	15.638	2130	2136	2145	rBV	295268	441492	15.74%	1.987%
27	15.768	2154	2158	2162	rVB5	4672	7212	0.26%	0.032%
28	16.208	2230	2233	2236	rVB2	1855	2975	0.11%	0.013%
29	17.049	2372	2376	2377	rBV4	2226	3149	0.11%	0.014%
30	17.278	2408	2415	2424	rBV	881571	1362358	48.57%	6.132%
31	17.372	2424	2431	2441	rVV	1323045	1988555	70.90%	8.950%
32	17.942	2525	2528	2533	rBV3	2914	4586	0.16%	0.021%
33	18.171	2562	2567	2569	rBV3	9094	11550	0.41%	0.052%
34	18.923	2694	2695	2701	rBV6	3678	4804	0.17%	0.022%
35	19.228	2743	2747	2751	rBV2	19516	29039	1.04%	0.131%
36	19.299	2755	2759	2764	rVB	19368	26238	0.94%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062707.D
 Acq On : 10 Sep 2024 18:55
 Operator : JU/RC
 Sample : P3843-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHJM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	19.598	2805	2810	2814	rBV5	8521	11169	0.40%	0.050%
38	19.663	2815	2821	2828	rBV	1870135	2695664	96.11%	12.133%
39	19.851	2849	2853	2857	rBV6	6177	10887	0.39%	0.049%
40	20.280	2921	2926	2928	rBV6	6370	10820	0.39%	0.049%
41	20.427	2949	2951	2954	rBV4	5056	5128	0.18%	0.023%
42	20.691	2994	2996	2997	rBV	5632	3481	0.12%	0.016%
43	21.520	3130	3137	3149	rBV	1180385	1831268	65.29%	8.242%
44	22.654	3328	3330	3333	rBV4	5446	7144	0.25%	0.032%
45	22.965	3377	3383	3388	rBV4	15714	28747	1.02%	0.129%
46	23.723	3507	3512	3518	rVB5	20579	39922	1.42%	0.180%
47	24.087	3572	3574	3577	rBV4	5300	4903	0.17%	0.022%
48	24.375	3611	3623	3636	rBV	1079868	2804719	100.00%	12.624%
49	24.581	3647	3658	3675	rBV	698365	1951227	69.57%	8.782%
50	24.745	3684	3686	3688	rVB3	8725	6347	0.23%	0.029%
51	24.975	3723	3725	3727	rBV3	5511	6329	0.23%	0.028%
52	25.210	3763	3765	3767	rBV3	5750	3713	0.13%	0.017%
53	25.668	3840	3843	3844	rBV3	10133	10734	0.38%	0.048%
54	26.379	3962	3964	3966	rVB3	5544	4231	0.15%	0.019%
55	26.655	4009	4011	4014	rBV4	4785	4577	0.16%	0.021%
56	26.913	4054	4055	4056	rBV	7231	3700	0.13%	0.017%
57	26.943	4056	4060	4072	rVB	18822	52703	1.88%	0.237%
58	28.306	4290	4292	4297	rBV6	4313	5294	0.19%	0.024%
59	28.470	4312	4320	4321	rBV6	16340	35216	1.26%	0.159%
60	30.251	4622	4623	4624	rBV	6173	2992	0.11%	0.013%
61	30.286	4627	4629	4630	rBV2	5407	3596	0.13%	0.016%
62	30.738	4704	4706	4707	rVB2	5150	3151	0.11%	0.014%
63	30.750	4707	4708	4711	rBV3	5266	6019	0.21%	0.027%
64	32.131	4941	4943	4944	rBV2	5508	3315	0.12%	0.015%
65	32.190	4951	4953	4954	rBV2	4151	3731	0.13%	0.017%
66	32.530	5009	5011	5012	rBV2	5323	3468	0.12%	0.016%




Sum of corrected areas: 22217903

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062707.D
Acq On : 10 Sep 2024 18:55
Operator : JU/RC
Sample : P3843-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

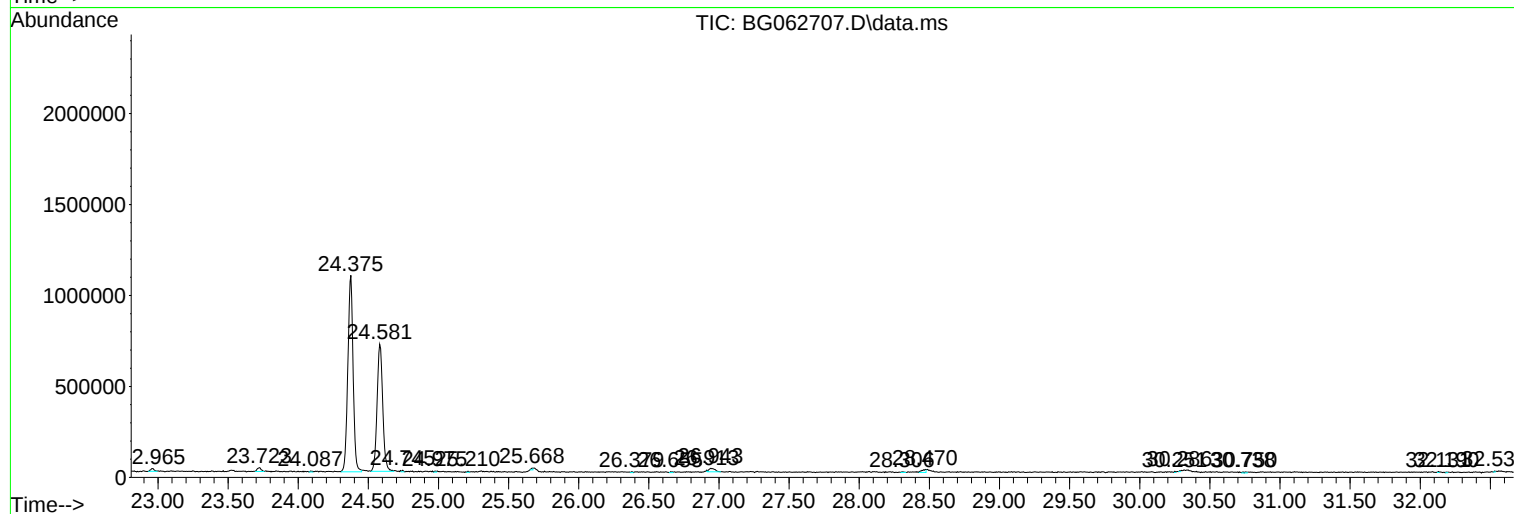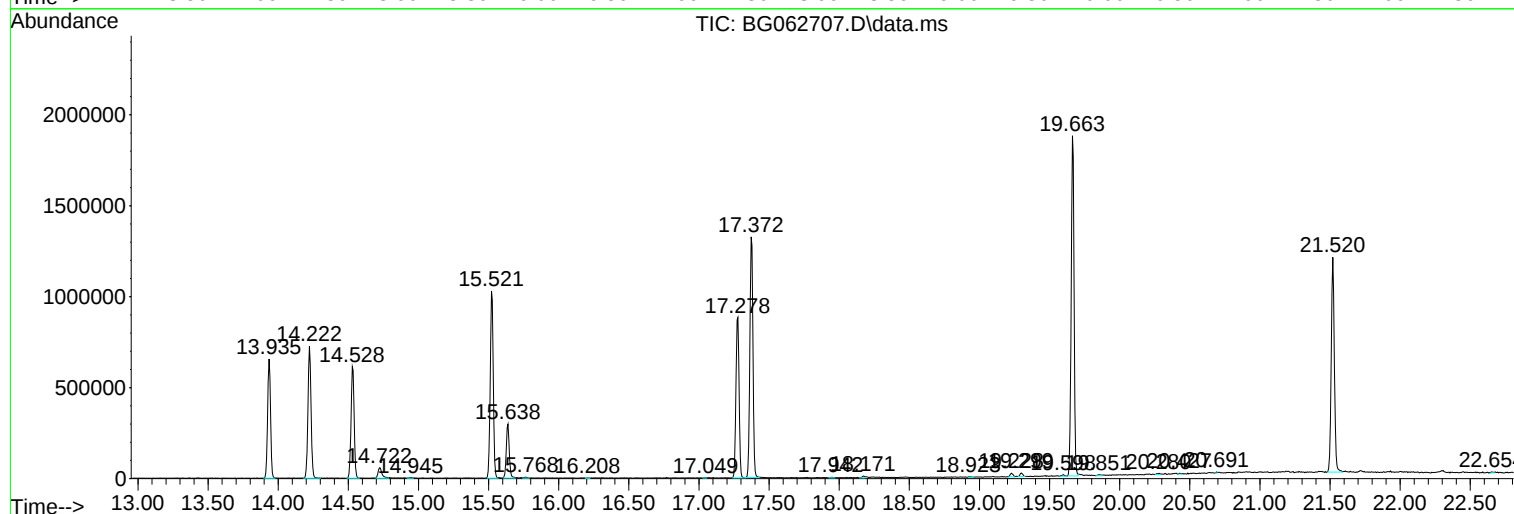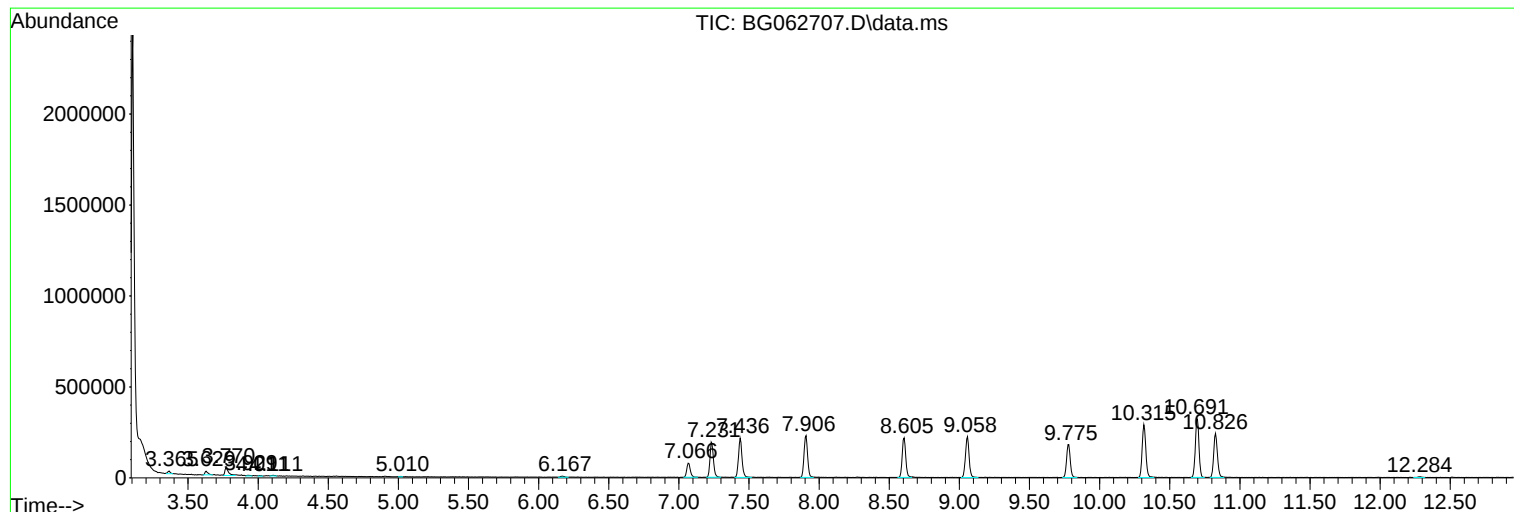

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062707.D
Acq On : 10 Sep 2024 18:55
Operator : JU/RC
Sample : P3843-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062707.D
Acq On : 10 Sep 2024 18:55
Operator : JU/RC
Sample : P3843-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHJM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc