

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062719.D
 Acq On : 11 Sep 2024 3:43
 Operator : JU/RC
 Sample : PB163242BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.360	42	46	51	rVB3	13912	20887	0.92%	0.108%
2	3.766	111	115	128	rBV	176365	317685	14.03%	1.649%
3	3.995	151	154	159	rBV6	2391	5236	0.23%	0.027%
4	4.106	170	173	174	rBV3	3290	3335	0.15%	0.017%
5	4.700	272	274	278	rVB2	2281	2548	0.11%	0.013%
6	5.005	325	326	330	rVB4	2178	2303	0.10%	0.012%
7	6.222	529	533	537	rBV4	1409	2874	0.13%	0.015%
8	7.068	670	677	688	rBV	191888	320281	14.15%	1.662%
9	7.232	698	705	713	rBV	144968	238504	10.53%	1.238%
10	7.432	733	739	748	rVB	172976	305302	13.48%	1.584%
11	7.902	813	819	827	rBV	191660	322400	14.24%	1.673%
12	8.601	931	938	948	rBV	241511	410845	18.15%	2.132%
13	9.054	1006	1015	1022	rBV	178058	302598	13.36%	1.570%
14	9.776	1131	1138	1147	rBV	154298	273826	12.09%	1.421%
15	10.311	1223	1229	1240	rBV	229399	402483	17.78%	2.089%
16	10.693	1287	1294	1302	rBV	272442	479992	21.20%	2.491%
17	10.822	1308	1316	1328	rBV	221909	405537	17.91%	2.104%
18	12.279	1560	1564	1568	rBV3	3063	5137	0.23%	0.027%
19	13.930	1839	1845	1855	rBV	527166	776566	34.30%	4.030%
20	14.224	1886	1895	1905	rBV	570610	900642	39.78%	4.674%
21	14.529	1937	1947	1955	rBV	543918	830359	36.67%	4.309%
22	14.723	1974	1980	1991	rBV	243909	396694	17.52%	2.059%
23	14.811	1993	1995	1998	rVB3	2352	2818	0.12%	0.015%
24	15.522	2108	2116	2127	rBV	827711	1253083	55.35%	6.503%
25	15.634	2129	2135	2149	rVB	265979	386060	17.05%	2.003%
26	15.763	2152	2157	2161	rVB2	3910	5874	0.26%	0.030%
27	17.273	2407	2414	2424	rBV	852028	1232764	54.45%	6.397%
28	17.373	2424	2431	2443	rVB	1101239	1562152	69.00%	8.106%
29	17.949	2522	2529	2530	rBV3	1668	2791	0.12%	0.014%
30	19.224	2743	2746	2750	rBV3	14440	18916	0.84%	0.098%
31	19.294	2753	2758	2763	rBV2	12784	18647	0.82%	0.097%
32	19.418	2776	2779	2783	rBV3	1375	2339	0.10%	0.012%
33	19.665	2814	2821	2834	rBV	1482626	2163737	95.57%	11.228%
34	19.882	2856	2858	2862	rVB2	2050	2384	0.11%	0.012%
35	19.917	2862	2864	2867	rBV3	2602	2652	0.12%	0.014%
36	20.634	2983	2986	2990	rBV4	4257	6911	0.31%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062719.D
 Acq On : 11 Sep 2024 3:43
 Operator : JU/RC
 Sample : PB163242BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	20.687	2994	2995	2997	rBV2	3000	2693	0.12%	0.014%
38	20.957	3039	3041	3043	rBV3	3681	3262	0.14%	0.017%
39	21.515	3129	3136	3149	rBV2	1057902	1700383	75.10%	8.824%
40	21.780	3178	3181	3184	rBV5	2873	3637	0.16%	0.019%
41	21.991	3215	3217	3218	rBV2	4014	3577	0.16%	0.019%
42	22.955	3377	3381	3388	rVB5	10862	19496	0.86%	0.101%
43	23.695	3505	3507	3508	rBV2	5408	5300	0.23%	0.028%
44	23.719	3508	3511	3516	rVB6	11775	19728	0.87%	0.102%
45	23.924	3544	3546	3548	rBV3	3403	2809	0.12%	0.015%
46	24.371	3611	3622	3637	rBV2	858783	2264122	100.00%	11.749%
47	24.577	3646	3657	3672	rVB	644484	1782672	78.74%	9.251%
48	25.663	3837	3842	3852	rVB9	15339	40507	1.79%	0.210%
49	25.769	3858	3860	3861	rBV2	3171	2450	0.11%	0.013%
50	26.933	4051	4058	4059	rBV6	12577	20140	0.89%	0.105%
51	29.394	4476	4477	4479	rBV2	4169	2701	0.12%	0.014%
52	29.888	4559	4561	4563	rBV3	4239	2832	0.13%	0.015%
53	30.487	4662	4663	4666	rVB3	3477	2267	0.10%	0.012%
54	31.098	4765	4767	4768	rBV2	3494	2516	0.11%	0.013%
55	32.273	4965	4967	4969	rBV3	3934	2280	0.10%	0.012%




Sum of corrected areas: 19270534

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062719.D
Acq On : 11 Sep 2024 3:43
Operator : JU/RC
Sample : PB163242BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

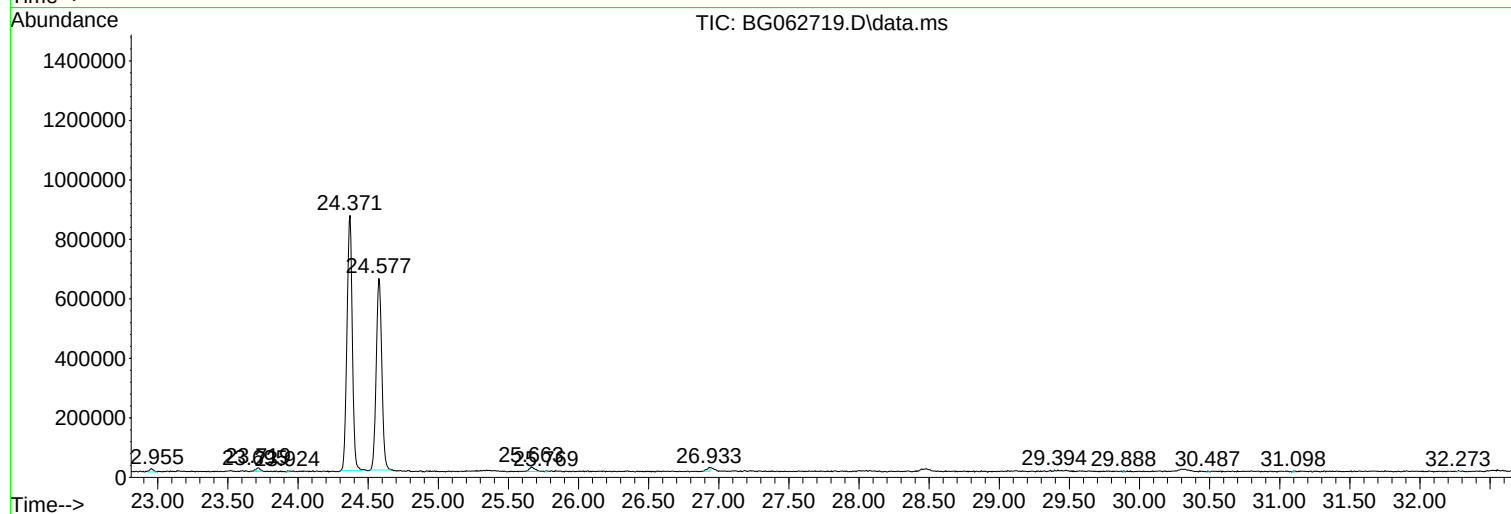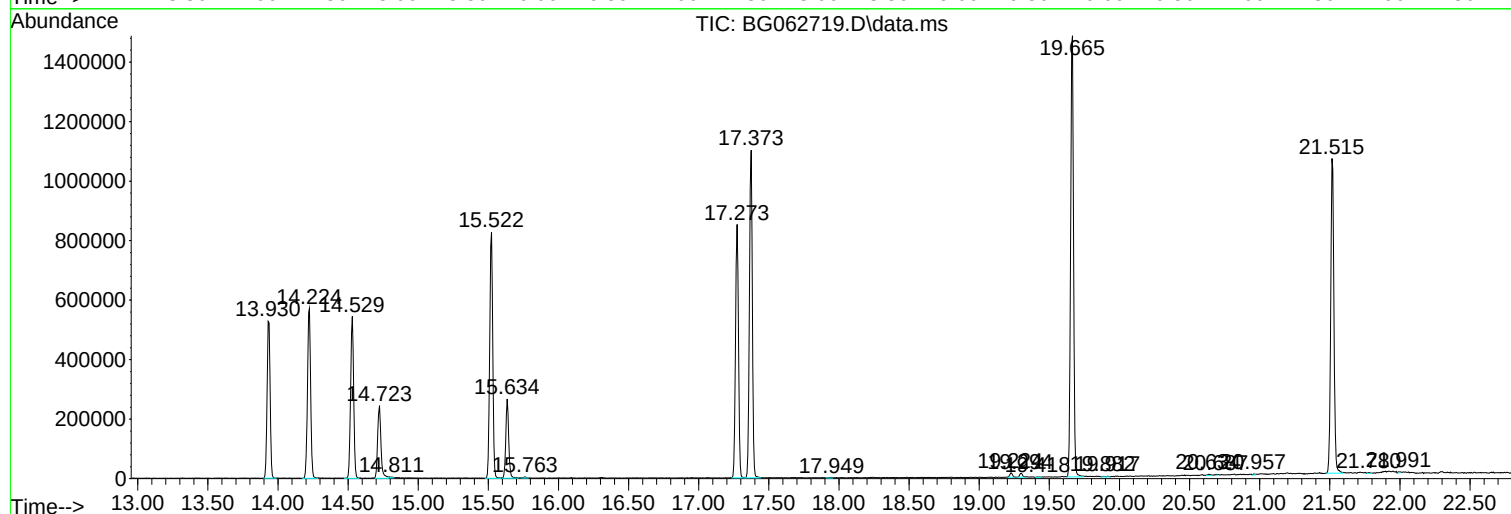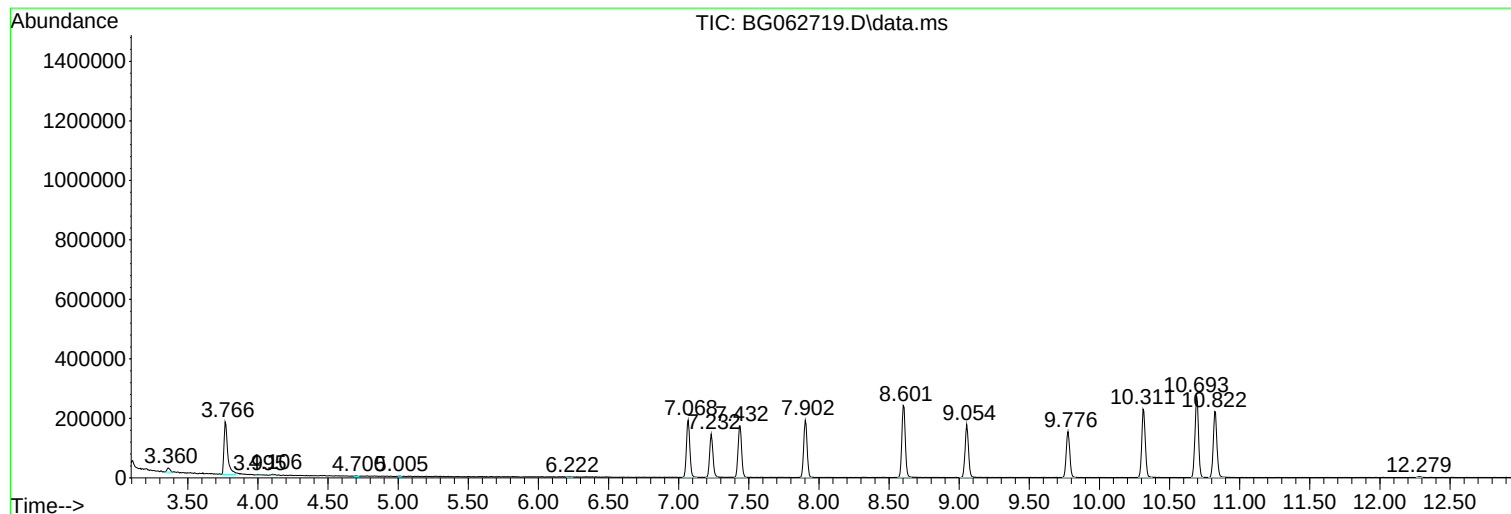

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062719.D
Acq On : 11 Sep 2024 3:43
Operator : JU/RC
Sample : PB163242BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062719.D
Acq On : 11 Sep 2024 3:43
Operator : JU/RC
Sample : PB163242BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc