

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062720.D
 Acq On : 11 Sep 2024 4:24
 Operator : JU/RC
 Sample : PB163193BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK193

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	43	47	53	rVB3	14029	20716	0.88%	0.106%
2	3.710	104	106	110	rVB5	2742	2739	0.12%	0.014%
3	3.769	111	116	131	rBV	182408	329998	14.01%	1.689%
4	4.104	170	173	180	rBV5	3829	7326	0.31%	0.037%
5	4.192	186	188	193	rBV6	2727	3454	0.15%	0.018%
6	4.298	204	206	210	rVB4	3009	3055	0.13%	0.016%
7	4.392	221	222	225	rBV2	2547	2407	0.10%	0.012%
8	7.065	670	677	692	rBV	236871	409343	17.37%	2.095%
9	7.235	699	706	716	rBV	180470	311400	13.22%	1.594%
10	7.435	734	740	748	rVB	234669	391203	16.60%	2.002%
11	7.905	813	820	828	rBV	171153	299439	12.71%	1.532%
12	8.604	932	939	949	rBV	258387	427511	18.15%	2.188%
13	9.051	1007	1015	1023	rBV	178680	322167	13.67%	1.649%
14	9.774	1132	1138	1147	rBV	152220	267710	11.36%	1.370%
15	10.314	1222	1230	1241	rBV	238645	418511	17.76%	2.142%
16	10.696	1285	1295	1305	rBV	259176	451996	19.18%	2.313%
17	10.825	1310	1317	1329	rVV	238112	420555	17.85%	2.152%
18	10.925	1332	1334	1338	rVB3	1869	2377	0.10%	0.012%
19	12.282	1561	1565	1567	rBV2	3034	4012	0.17%	0.021%
20	13.933	1840	1846	1858	rVB	564874	799313	33.93%	4.090%
21	14.221	1888	1895	1906	rBV	593389	913698	38.78%	4.676%
22	14.527	1940	1947	1954	rBV	489857	753098	31.97%	3.854%
23	14.721	1973	1980	1994	rBV	251033	416790	17.69%	2.133%
24	15.520	2109	2116	2123	rBV	846993	1280916	54.37%	6.555%
25	15.637	2130	2136	2147	rBV	273545	397193	16.86%	2.033%
26	15.761	2153	2157	2162	rVB5	3302	4970	0.21%	0.025%
27	16.307	2245	2250	2254	rVB3	2366	4292	0.18%	0.022%
28	17.277	2408	2415	2421	rBV	759426	1128238	47.89%	5.774%
29	17.371	2424	2431	2442	rVV	1088578	1606093	68.17%	8.219%
30	19.227	2743	2747	2751	rBV2	15224	21129	0.90%	0.108%
31	19.298	2754	2759	2763	rBV2	13931	19412	0.82%	0.099%
32	19.597	2806	2810	2814	rVB3	8469	9529	0.40%	0.049%
33	19.662	2814	2821	2833	rBV	1613443	2265040	96.14%	11.591%
34	19.991	2873	2877	2879	rVB4	2537	2761	0.12%	0.014%
35	20.038	2883	2885	2888	rBV3	1982	2464	0.10%	0.013%
36	20.261	2920	2923	2927	rBV3	2214	4199	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062720.D
 Acq On : 11 Sep 2024 4:24
 Operator : JU/RC
 Sample : PB163193BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK193

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	20.437	2949	2953	2955	rBV4	3243	3978	0.17%	0.020%
38	20.637	2984	2987	2990	rVB5	9723	10926	0.46%	0.056%
39	21.266	3092	3094	3096	rBV3	3288	3469	0.15%	0.018%
40	21.519	3130	3137	3151	rBV	990105	1564799	66.42%	8.008%
41	21.677	3162	3164	3166	rVB3	3573	2415	0.10%	0.012%
42	21.724	3168	3172	3175	rVB3	4825	7569	0.32%	0.039%
43	22.294	3267	3269	3273	rVB4	7289	9674	0.41%	0.050%
44	22.635	3325	3327	3329	rBV3	3371	2870	0.12%	0.015%
45	22.958	3378	3382	3389	rVB4	12390	22669	0.96%	0.116%
46	23.722	3506	3512	3518	rVB5	17862	34000	1.44%	0.174%
47	24.374	3612	3623	3640	rBV2	897729	2355997	100.00%	12.057%
48	24.580	3647	3658	3673	rBV	602436	1660896	70.50%	8.500%
49	25.678	3836	3845	3853	rBV7	20935	60981	2.59%	0.312%
50	25.837	3871	3872	3875	rBV3	4972	3601	0.15%	0.018%
51	26.513	3986	3987	3990	rBV3	4048	3236	0.14%	0.017%
52	26.942	4053	4060	4069	rVB7	17517	54741	2.32%	0.280%
53	28.734	4363	4365	4367	rBV3	2938	2679	0.11%	0.014%
54	28.975	4403	4406	4408	rBV4	4651	5593	0.24%	0.029%
55	32.523	5008	5010	5012	rBV3	4847	5915	0.25%	0.030%




Sum of corrected areas: 19541062

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062720.D
Acq On : 11 Sep 2024 4:24
Operator : JU/RC
Sample : PB163193BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

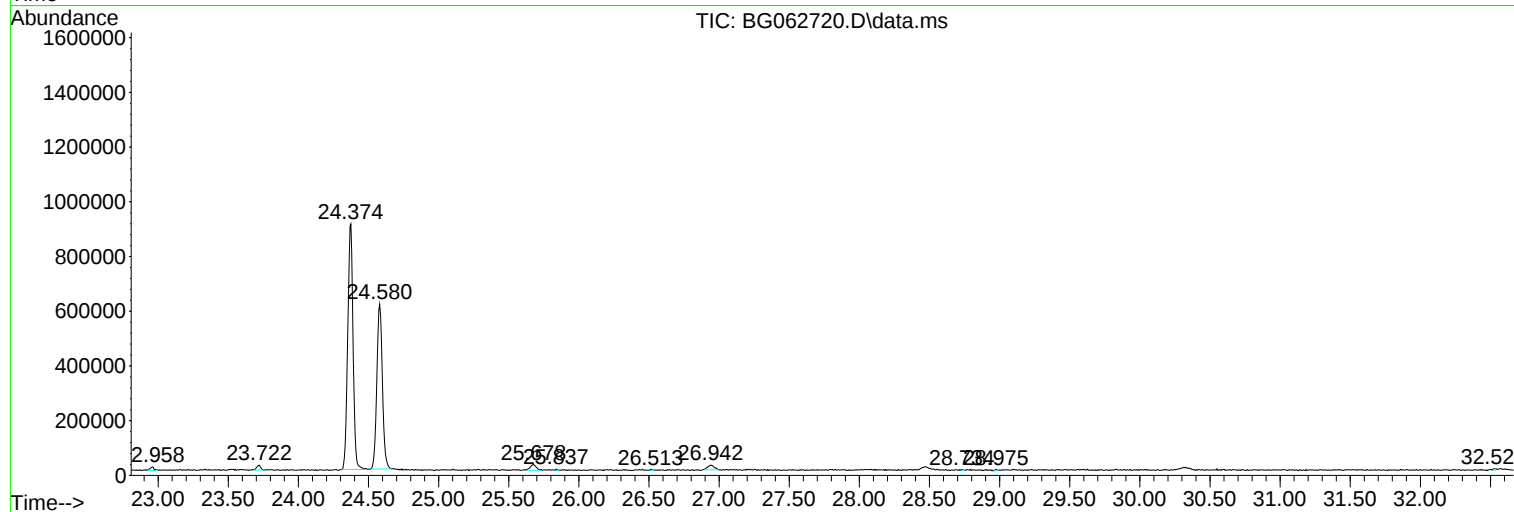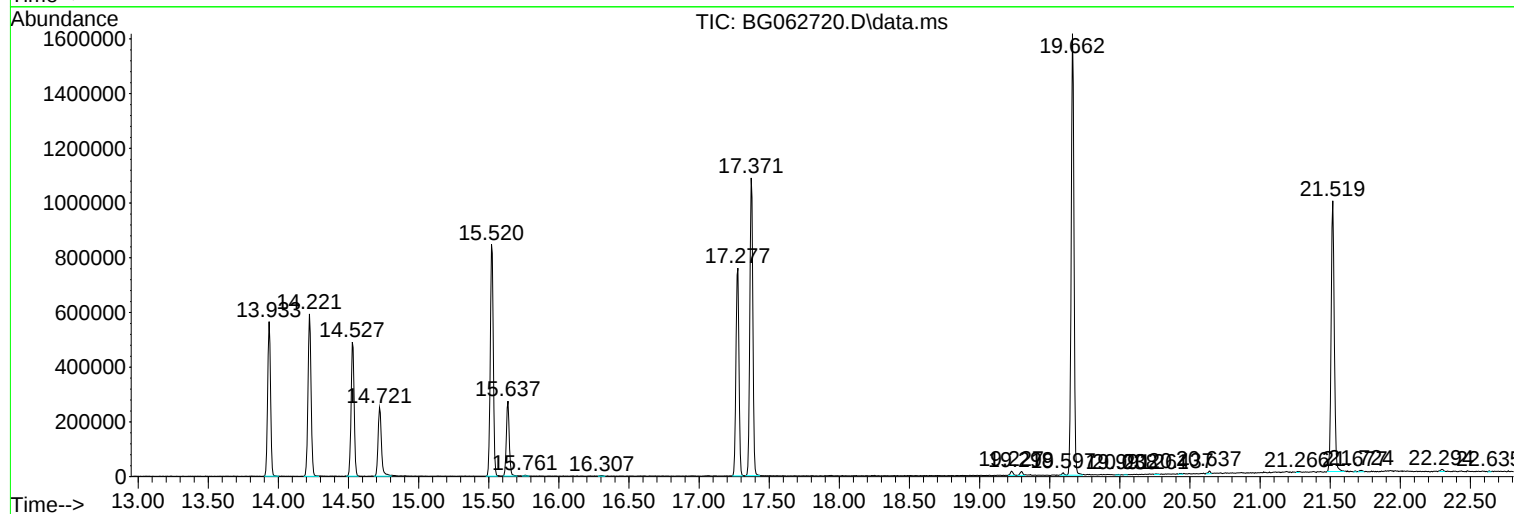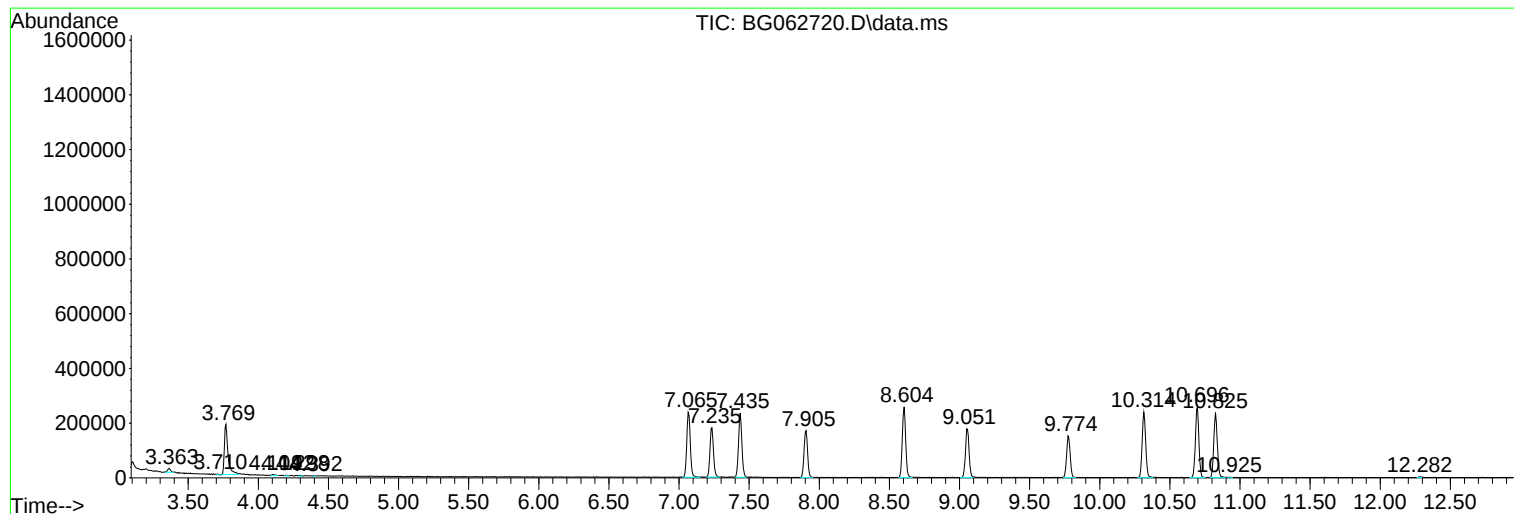

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062720.D
Acq On : 11 Sep 2024 4:24
Operator : JU/RC
Sample : PB163193BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062720.D
Acq On : 11 Sep 2024 4:24
Operator : JU/RC
Sample : PB163193BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc