

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062721.D
 Acq On : 11 Sep 2024 5:04
 Operator : JU/RC
 Sample : P3878-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDCG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	44	47	51	rVB	9989	12191	0.46%	0.061%
2	3.775	113	117	125	rBV	25702	44876	1.70%	0.226%
3	4.104	170	173	179	rVB4	6624	11395	0.43%	0.057%
4	4.557	247	250	253	rBV3	2071	2990	0.11%	0.015%
5	4.909	306	310	313	rVB4	3401	4127	0.16%	0.021%
6	5.021	323	329	331	rBV4	3739	5270	0.20%	0.027%
7	5.579	419	424	428	rVB6	2860	5492	0.21%	0.028%
8	6.166	518	524	529	rVB6	5889	8801	0.33%	0.044%
9	7.065	671	677	686	rBV	54247	90604	3.42%	0.456%
10	7.230	697	705	715	rBV	148023	255751	9.67%	1.286%
11	7.436	734	740	749	rBV	171696	290787	10.99%	1.462%
12	7.906	813	820	827	rBV	199815	339501	12.83%	1.707%
13	7.964	827	830	834	rVB3	4782	6832	0.26%	0.034%
14	8.605	932	939	948	rBV	158252	275414	10.41%	1.385%
15	9.057	1007	1016	1026	rBV	181326	328022	12.40%	1.649%
16	9.774	1132	1138	1149	rBV	151403	270330	10.22%	1.359%
17	10.314	1222	1230	1237	rBV	235668	414000	15.65%	2.082%
18	10.696	1287	1295	1305	rVB	283537	506250	19.13%	2.546%
19	10.826	1310	1317	1331	rBV	157670	285852	10.80%	1.437%
20	12.283	1560	1565	1570	rBV3	3580	6771	0.26%	0.034%
21	12.506	1600	1603	1608	rBV2	2436	3947	0.15%	0.020%
22	13.934	1839	1846	1853	rBV	608565	831798	31.44%	4.183%
23	14.222	1887	1895	1903	rBV	644122	950188	35.91%	4.778%
24	14.527	1940	1947	1957	rBV	567498	866190	32.73%	4.356%
25	14.721	1973	1980	1990	rBV2	59771	110156	4.16%	0.554%
26	15.520	2110	2116	2123	rBV	941603	1382635	52.25%	6.953%
27	15.638	2129	2136	2146	rBV	300072	455043	17.20%	2.288%
28	17.060	2374	2378	2383	rVB4	1538	2726	0.10%	0.014%
29	17.271	2408	2414	2424	rBV	862064	1285941	48.60%	6.466%
30	17.371	2424	2431	2444	rVV2	1288331	1872693	70.77%	9.417%
31	17.812	2502	2506	2509	rVB3	2200	3006	0.11%	0.015%
32	17.941	2526	2528	2533	rVB2	2654	2841	0.11%	0.014%
33	18.235	2575	2578	2582	rVB4	2200	2919	0.11%	0.015%
34	19.228	2743	2747	2752	rVB4	18008	25515	0.96%	0.128%
35	19.298	2754	2759	2767	rVV	17717	26938	1.02%	0.135%
36	19.521	2793	2797	2799	rBV2	1821	2712	0.10%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062721.D
 Acq On : 11 Sep 2024 5:04
 Operator : JU/RC
 Sample : P3878-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDCG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	19.592	2802	2809	2813	rBV5	4721	9099	0.34%	0.046%
38	19.662	2814	2821	2833	rBV	1784663	2558288	96.68%	12.864%
39	20.473	2958	2959	2964	rBV4	2077	3265	0.12%	0.016%
40	20.638	2985	2987	2990	rVB3	5549	4763	0.18%	0.024%
41	21.278	3094	3096	3099	rVB4	3514	2686	0.10%	0.014%
42	21.519	3130	3137	3153	rVB	1129498	1707893	64.54%	8.588%
43	21.848	3191	3193	3196	rVB4	3832	3259	0.12%	0.016%
44	22.018	3221	3222	3225	rBV3	3991	3227	0.12%	0.016%
45	22.653	3326	3330	3336	rVB4	23588	37435	1.41%	0.188%
46	22.953	3378	3381	3387	rVB7	7285	11811	0.45%	0.059%
47	23.052	3396	3398	3399	rBV2	4313	3178	0.12%	0.016%
48	23.246	3428	3431	3432	rBV3	3643	3575	0.14%	0.018%
49	23.587	3487	3489	3491	rBV3	3490	4029	0.15%	0.020%
50	23.716	3508	3511	3518	rVB7	8891	17634	0.67%	0.089%
51	23.922	3545	3546	3548	rBV2	5021	4227	0.16%	0.021%
52	24.374	3611	3623	3635	rBV	1005930	2646082	100.00%	13.306%
53	24.580	3647	3658	3677	rVB	647570	1802659	68.13%	9.065%
54	24.939	3717	3719	3723	rBV5	2752	4848	0.18%	0.024%
55	25.673	3836	3844	3854	rVB8	12861	41188	1.56%	0.207%
56	25.743	3854	3856	3857	rBV2	3060	2697	0.10%	0.014%
57	27.195	4101	4103	4104	rBV2	4554	3546	0.13%	0.018%
58	27.629	4175	4177	4178	rBV2	4264	4069	0.15%	0.020%
59	27.723	4190	4193	4195	rBV4	5187	5568	0.21%	0.028%
60	30.291	4628	4630	4631	rBV2	4104	2913	0.11%	0.015%
61	30.497	4661	4665	4669	rBV5	2987	4727	0.18%	0.024%
62	32.242	4960	4962	4964	rBV3	3301	3339	0.13%	0.017%




Sum of corrected areas: 19886509

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062721.D
Acq On : 11 Sep 2024 5:04
Operator : JU/RC
Sample : P3878-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDCG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

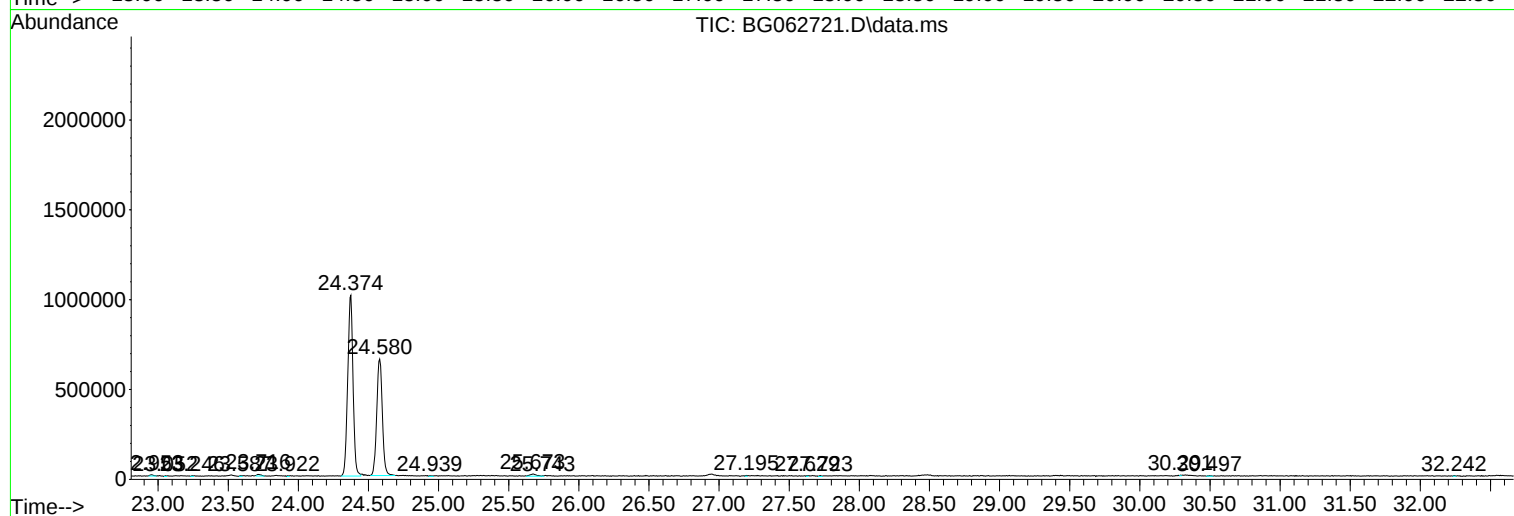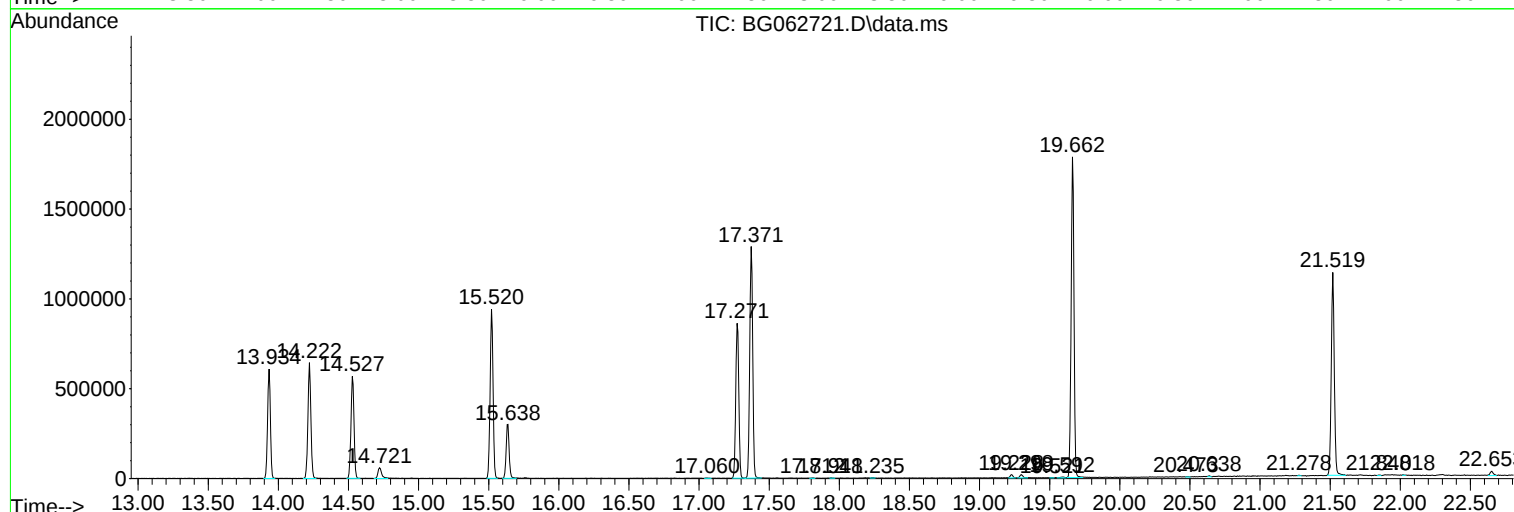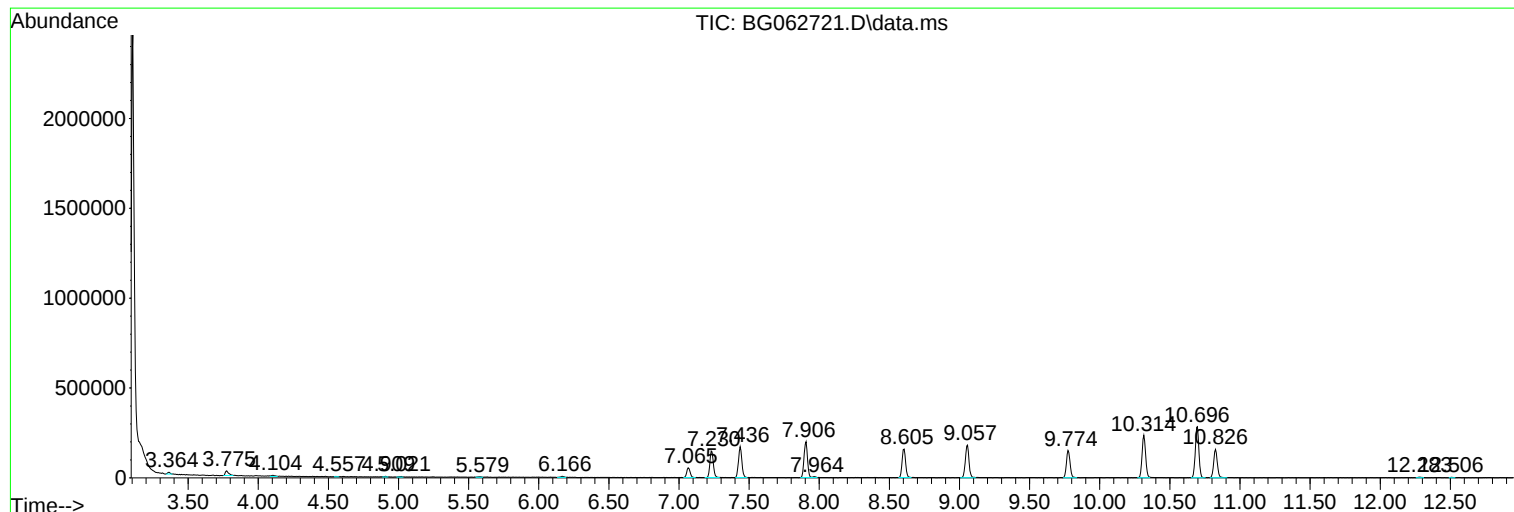

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062721.D
Acq On : 11 Sep 2024 5:04
Operator : JU/RC
Sample : P3878-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDCG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062721.D
Acq On : 11 Sep 2024 5:04
Operator : JU/RC
Sample : P3878-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDCG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc