

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062738.D
Acq On : 11 Sep 2024 16:27
Operator : JU/RC
Sample : P3877-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BG062738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.766	110	115	129	rVB	120036	207946	9.18%	1.023%
2	5.017	324	328	331	rVB3	2126	2569	0.11%	0.013%
3	6.997	661	665	667	rBV3	1897	2522	0.11%	0.012%
4	7.068	670	677	689	rVV	173770	301902	13.33%	1.485%
5	7.232	698	705	714	rBV	116488	196024	8.65%	0.964%
6	7.320	717	720	724	rBV4	1708	2278	0.10%	0.011%
7	7.432	733	739	747	rBV	164084	273170	12.06%	1.344%
8	7.902	812	819	826	rBV	295283	477271	21.07%	2.348%
9	7.961	826	829	838	rVB5	6789	11285	0.50%	0.056%
10	8.325	889	891	896	rVB4	2058	2301	0.10%	0.011%
11	8.601	930	938	948	rVV	220477	378509	16.71%	1.862%
12	9.054	1007	1015	1024	rBV	157557	273215	12.06%	1.344%
13	9.212	1034	1042	1044	rBV3	1681	3283	0.14%	0.016%
14	9.488	1083	1089	1094	rBV2	4591	6359	0.28%	0.031%
15	9.618	1105	1111	1116	rBV4	15102	25286	1.12%	0.124%
16	9.776	1128	1138	1145	rBV	135718	240032	10.59%	1.181%
17	10.023	1176	1180	1185	rBV4	1561	2764	0.12%	0.014%
18	10.317	1222	1230	1239	rBV	218419	394114	17.40%	1.939%
19	10.693	1287	1294	1302	rBV	407841	710879	31.38%	3.498%
20	10.828	1307	1317	1326	rBV	210116	388088	17.13%	1.909%
21	11.228	1381	1385	1392	rVB4	4760	6959	0.31%	0.034%
22	12.285	1560	1565	1567	rBV2	3673	5248	0.23%	0.026%
23	13.366	1743	1749	1755	rBV4	5463	8847	0.39%	0.044%
24	13.490	1765	1770	1778	rBV4	2205	4858	0.21%	0.024%
25	13.795	1818	1822	1825	rVB4	1829	2466	0.11%	0.012%
26	13.936	1839	1846	1853	rBV	448793	664007	29.31%	3.267%
27	14.224	1888	1895	1902	rVV	504263	802920	35.44%	3.951%
28	14.436	1927	1931	1936	rVB3	3625	4756	0.21%	0.023%
29	14.530	1940	1947	1954	rVV	818282	1223849	54.02%	6.022%
30	14.723	1972	1980	1991	rBV	184011	312602	13.80%	1.538%
31	14.953	2013	2019	2022	rBV4	3132	4034	0.18%	0.020%
32	15.158	2049	2054	2060	rVB5	7208	12898	0.57%	0.063%
33	15.329	2080	2083	2084	rBV	2559	2270	0.10%	0.011%
34	15.382	2089	2092	2097	rVB3	3583	4834	0.21%	0.024%
35	15.523	2109	2116	2124	rBV	755444	1131044	49.92%	5.565%
36	15.634	2130	2135	2144	rBV	167352	247138	10.91%	1.216%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
 Data File : BG062738.D
 Acq On : 11 Sep 2024 16:27
 Operator : JU/RC
 Sample : P3877-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCVZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	15.763	2151	2157	2160	rBV3	4230	7433	0.33%	0.037%
38	15.887	2173	2178	2183	rVB	65027	94898	4.19%	0.467%
39	15.946	2183	2188	2189	rBV3	2009	2720	0.12%	0.013%
40	16.310	2248	2250	2253	rVB3	2559	2565	0.11%	0.013%
41	16.592	2294	2298	2301	rVV3	1448	2553	0.11%	0.013%
42	16.774	2325	2329	2332	rVB4	1598	2466	0.11%	0.012%
43	16.927	2350	2355	2361	rBV2	52693	79635	3.51%	0.392%
44	17.033	2370	2373	2375	rBV3	3037	2583	0.11%	0.013%
45	17.074	2379	2380	2386	rVB5	2411	2442	0.11%	0.012%
46	17.197	2398	2401	2403	rVV3	2778	2579	0.11%	0.013%
47	17.273	2407	2414	2422	rVV	1163906	1780878	78.60%	8.762%
48	17.373	2424	2431	2442	rVV	981584	1401300	61.85%	6.895%
49	17.461	2442	2446	2451	rVB5	8087	11888	0.52%	0.058%
50	17.550	2460	2461	2465	rBV3	2289	2456	0.11%	0.012%
51	17.638	2475	2476	2479	rBV3	2928	2432	0.11%	0.012%
52	17.837	2508	2510	2514	rVB5	2311	3146	0.14%	0.015%
53	17.890	2514	2519	2524	rBV	38978	55852	2.47%	0.275%
54	17.943	2526	2528	2531	rVB4	3221	3380	0.15%	0.017%
55	18.049	2542	2546	2550	rBV4	2620	4275	0.19%	0.021%
56	18.119	2557	2558	2561	rBV3	2908	3396	0.15%	0.017%
57	18.166	2561	2566	2573	rBV3	76399	127995	5.65%	0.630%
58	18.237	2576	2578	2587	rVB8	6062	11662	0.51%	0.057%
59	18.354	2597	2598	2601	rVB3	3738	2624	0.12%	0.013%
60	18.472	2616	2618	2625	rVB8	4572	6682	0.29%	0.033%
61	18.695	2653	2656	2659	rBV4	3444	5410	0.24%	0.027%
62	18.731	2659	2662	2663	rBV3	4222	3532	0.16%	0.017%
63	18.742	2663	2664	2667	rVB3	3643	3176	0.14%	0.016%
64	18.772	2667	2669	2672	rBV4	3973	4544	0.20%	0.022%
65	18.895	2687	2690	2691	rVB3	3169	2891	0.13%	0.014%
66	18.913	2691	2693	2695	rBV2	2999	2990	0.13%	0.015%
67	19.230	2743	2747	2754	rVB4	17122	23047	1.02%	0.113%
68	19.300	2754	2759	2763	rBV3	18918	32933	1.45%	0.162%
69	19.447	2781	2784	2788	rBV6	14740	22430	0.99%	0.110%
70	19.600	2806	2810	2814	rVB7	8812	14064	0.62%	0.069%
71	19.665	2815	2821	2827	rBV	1279423	1788104	78.92%	8.798%
72	19.770	2836	2839	2841	rBV4	6871	7175	0.32%	0.035%
73	20.205	2911	2913	2916	rVB3	9248	8730	0.39%	0.043%
74	21.186	3076	3080	3088	rBV	126915	208305	9.19%	1.025%
75	21.521	3130	3137	3146	rVB	1347945	2105186	92.92%	10.358%
76	23.713	3506	3510	3516	rBV4	25649	53613	2.37%	0.264%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062738.D
Acq On : 11 Sep 2024 16:27
Operator : JU/RC
Sample : P3877-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Title : SVOA CALIBRATION

77	24.377	3613	3623	3633	rBV	661579	1720799	75.95%	8.467%
78	24.588	3649	3659	3676	rVB	816621	2265656	100.00%	11.147%
79	25.769	3857	3860	3861	rBV3	10585	12417	0.55%	0.061%
80	26.950	4054	4061	4072	rVB5	25775	78222	3.45%	0.385%
81	32.085	4933	4935	4936	rBV2	7252	4855	0.21%	0.024%


Sum of corrected areas: 20324446

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062738.D
Acq On : 11 Sep 2024 16:27
Operator : JU/RC
Sample : P3877-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

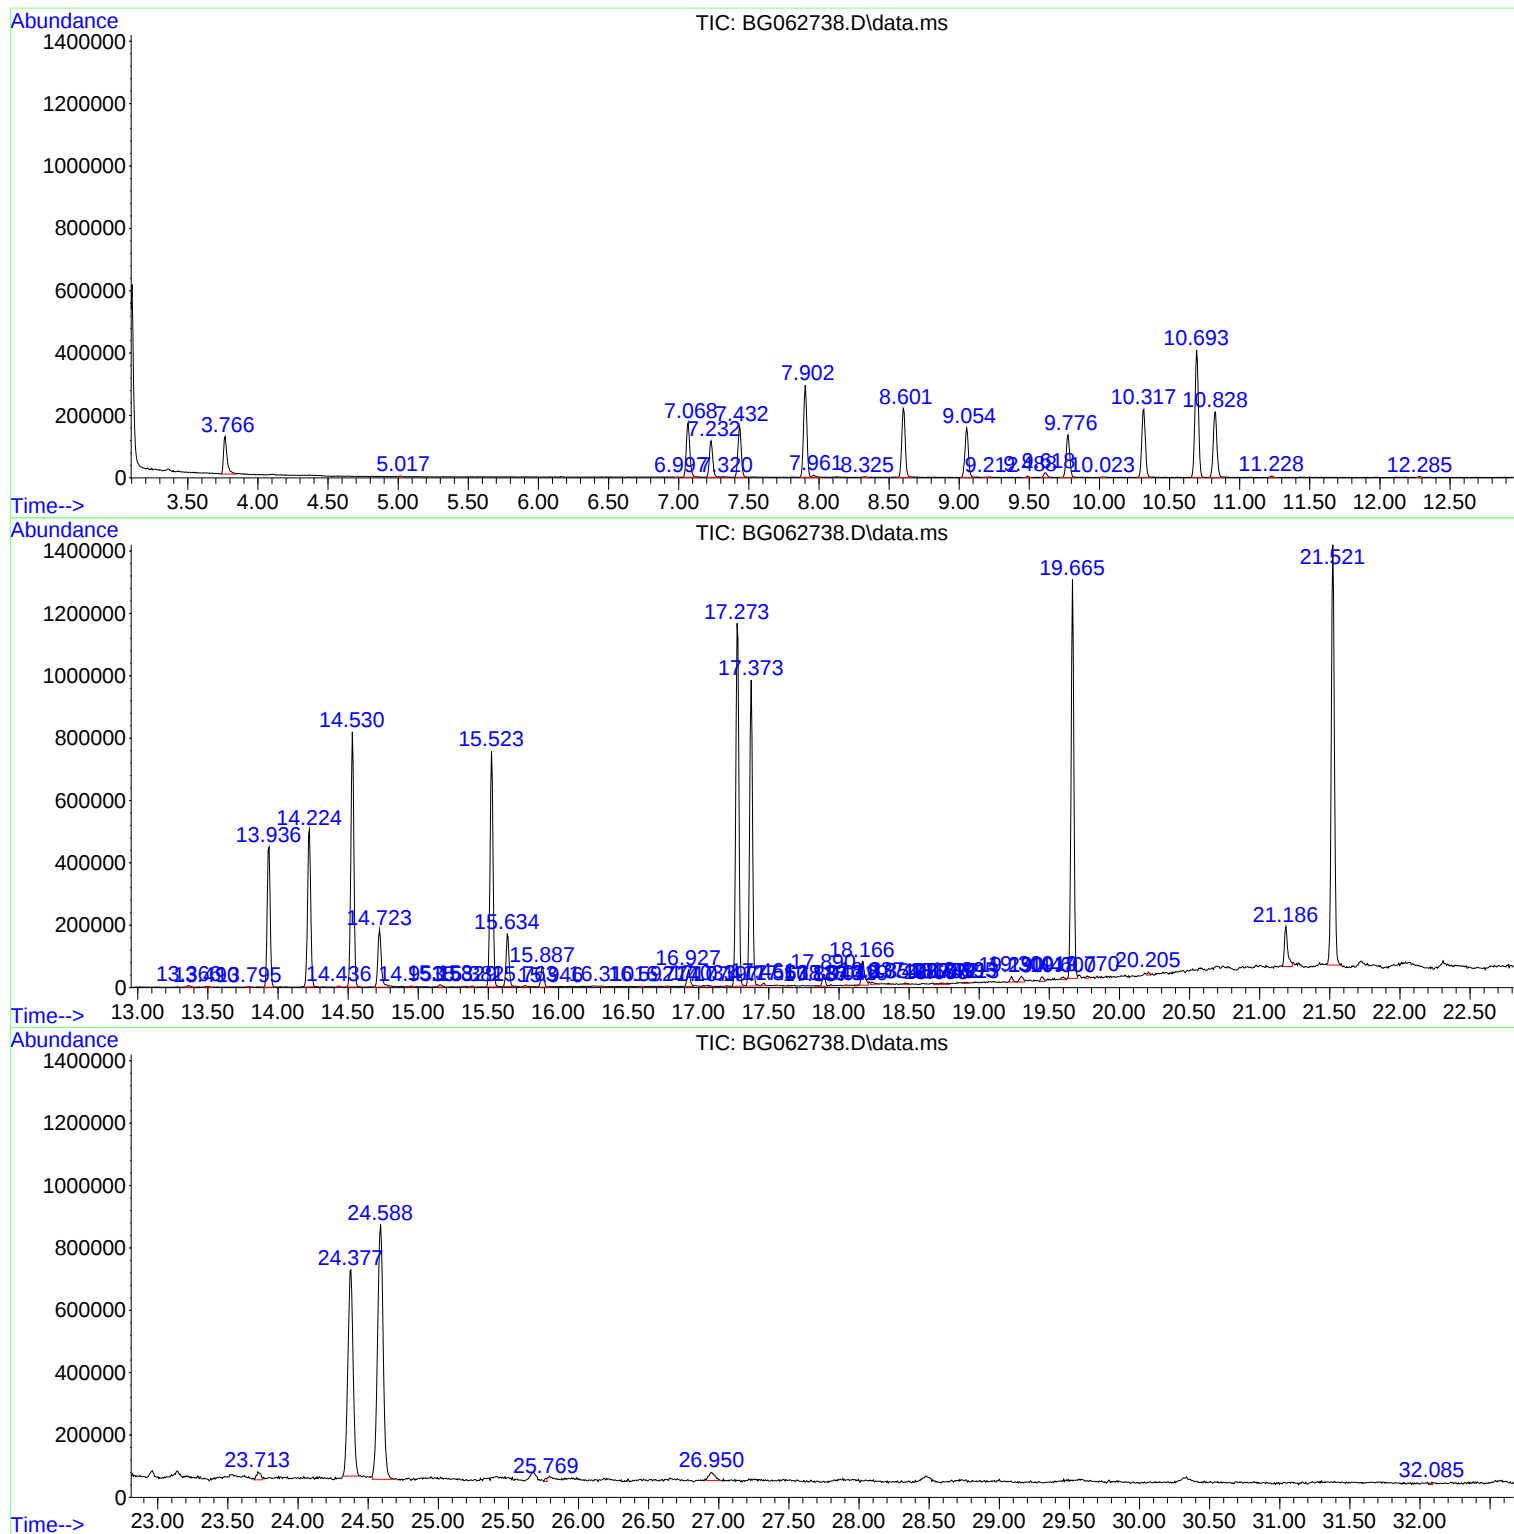

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062738.D
Acq On : 11 Sep 2024 16:27
Operator : JU/RC
Sample : P3877-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091024\
Data File : BG062738.D
Acq On : 11 Sep 2024 16:27
Operator : JU/RC
Sample : P3877-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc