
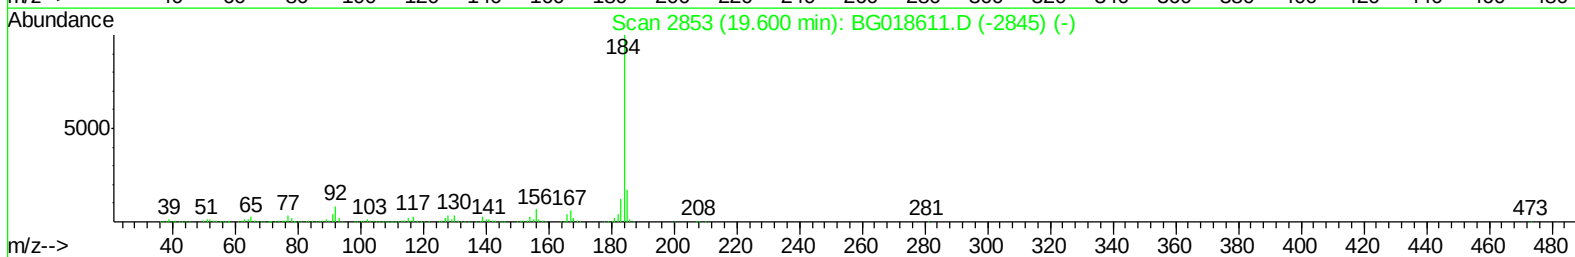
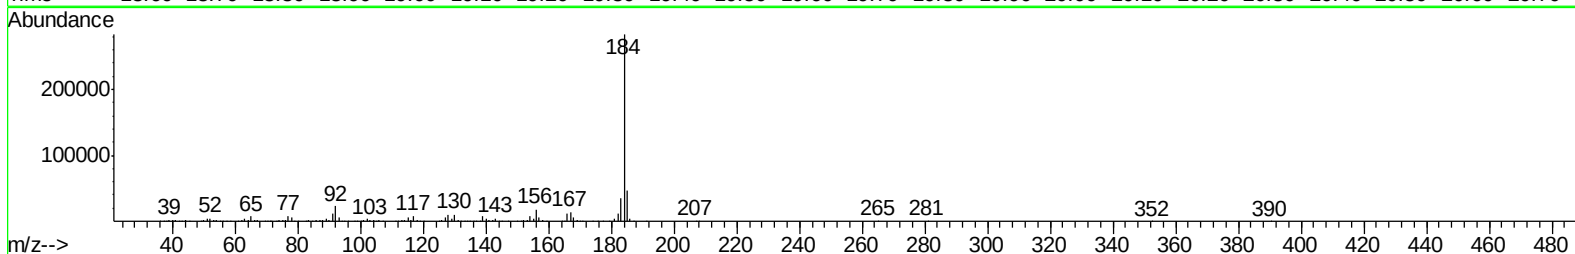


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091115\
 Data File : BG018607.D
 Acq On : 10 Sep 2015 17:59
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 11 02:25:30 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 11 01:56:11 2015
 Response via : Initial Calibration

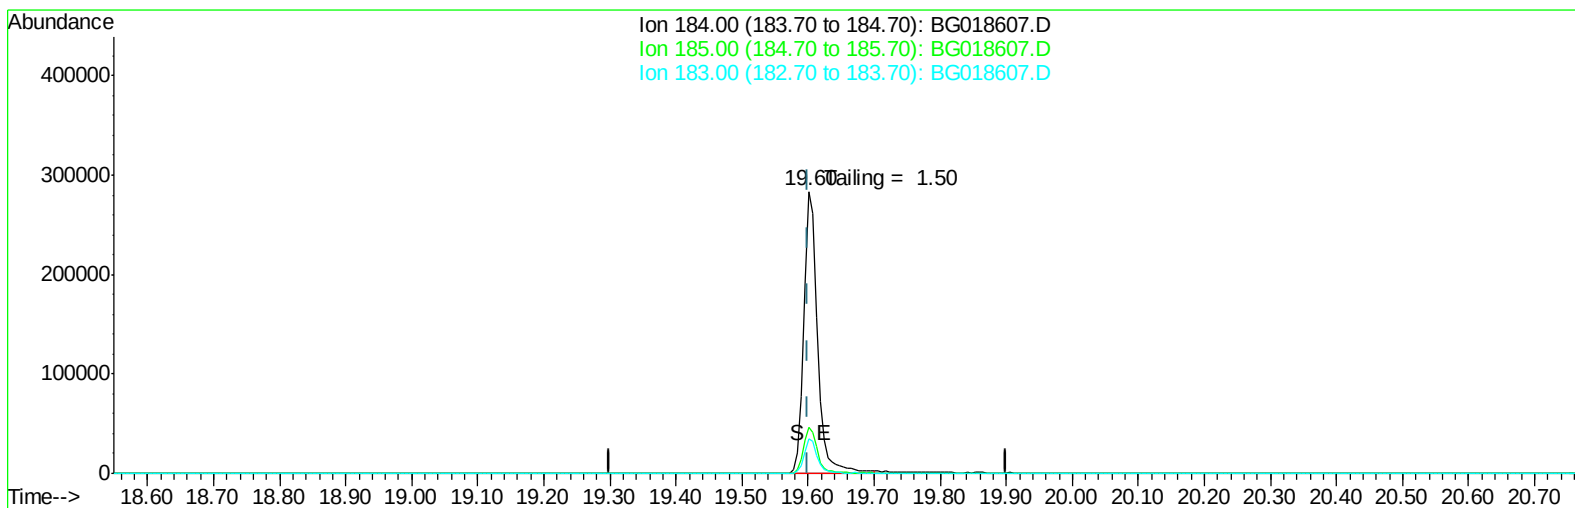

TIC: BG018607.D

(76) Benzidine




19.601min (+0.000) 173522.11ng

response 422081

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	16.38
183.00	12.60	12.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091115\
Data File : BG018607.D
Acq On : 10 Sep 2015 17:59
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 11 02:25:30 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 11 01:56:11 2015
Response via : Initial Calibration

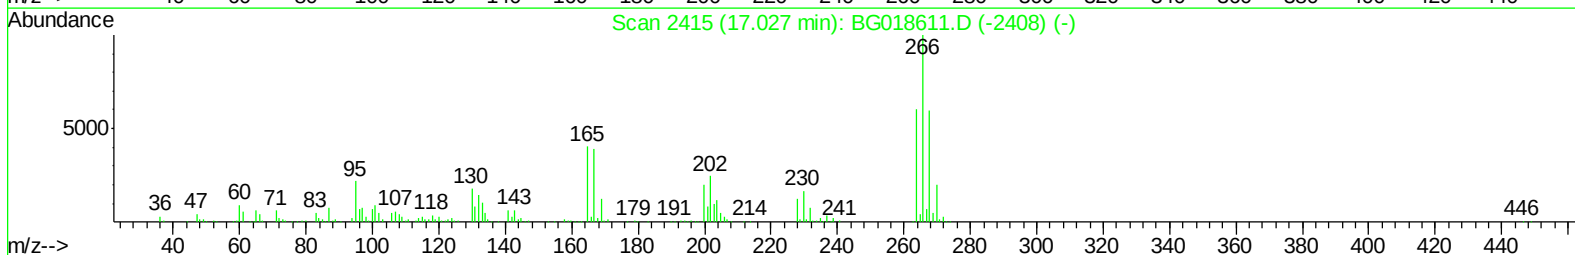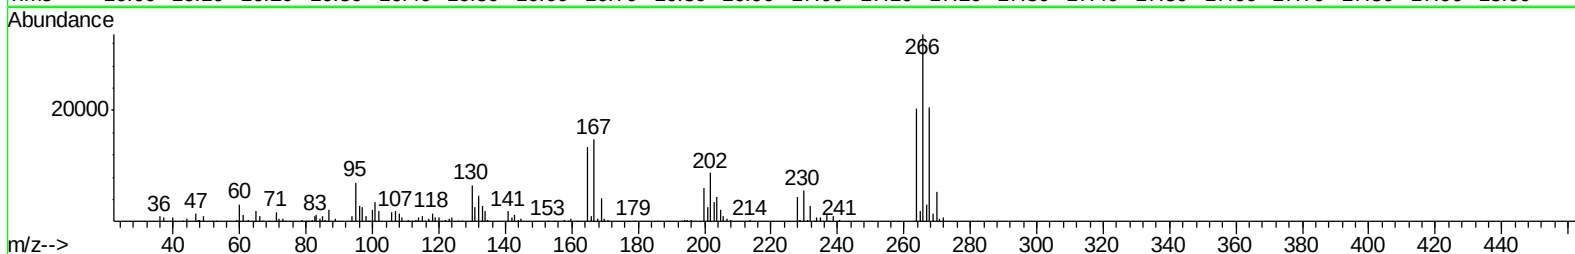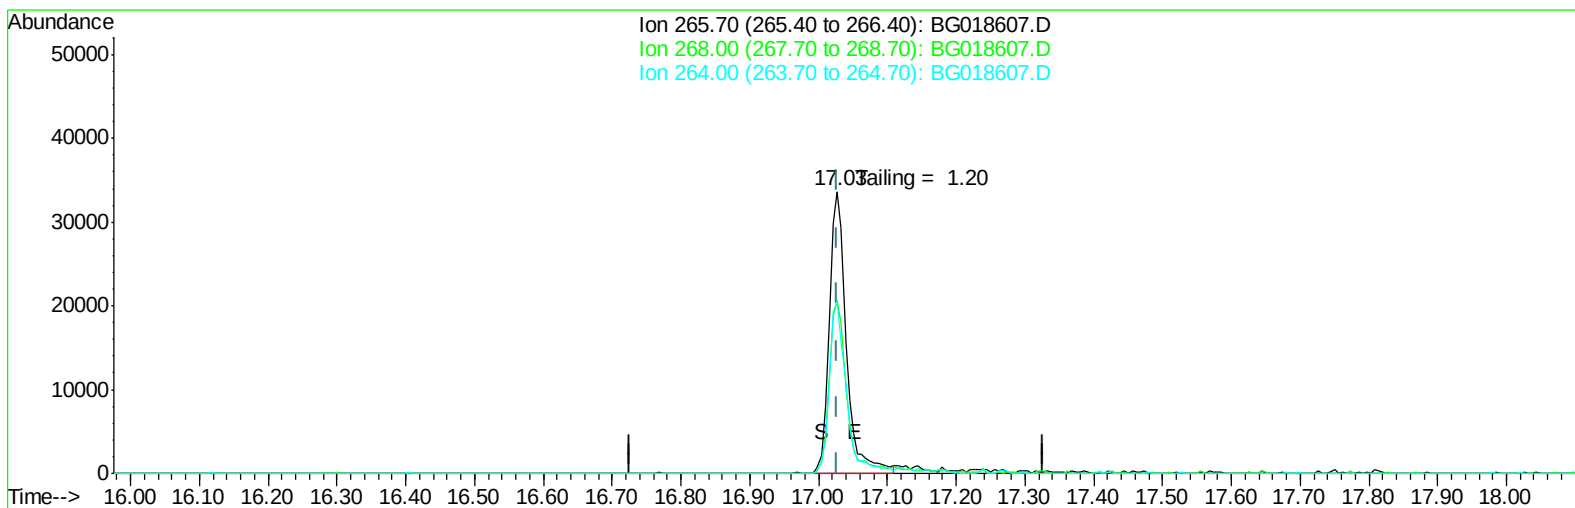

TIC: BG018607.D

(69) Pentachlorophenol (C)

17.027min (+0.000) 154214.75ng

response 57801

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	61.28
264.00	60.10	60.73
0.00	0.00	0.00