


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091115\  
 Data File : BG018607.D  
 Acq On : 10 Sep 2015 17:59  
 Operator : UM/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG091115.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Sep 11 10:44:16 2015

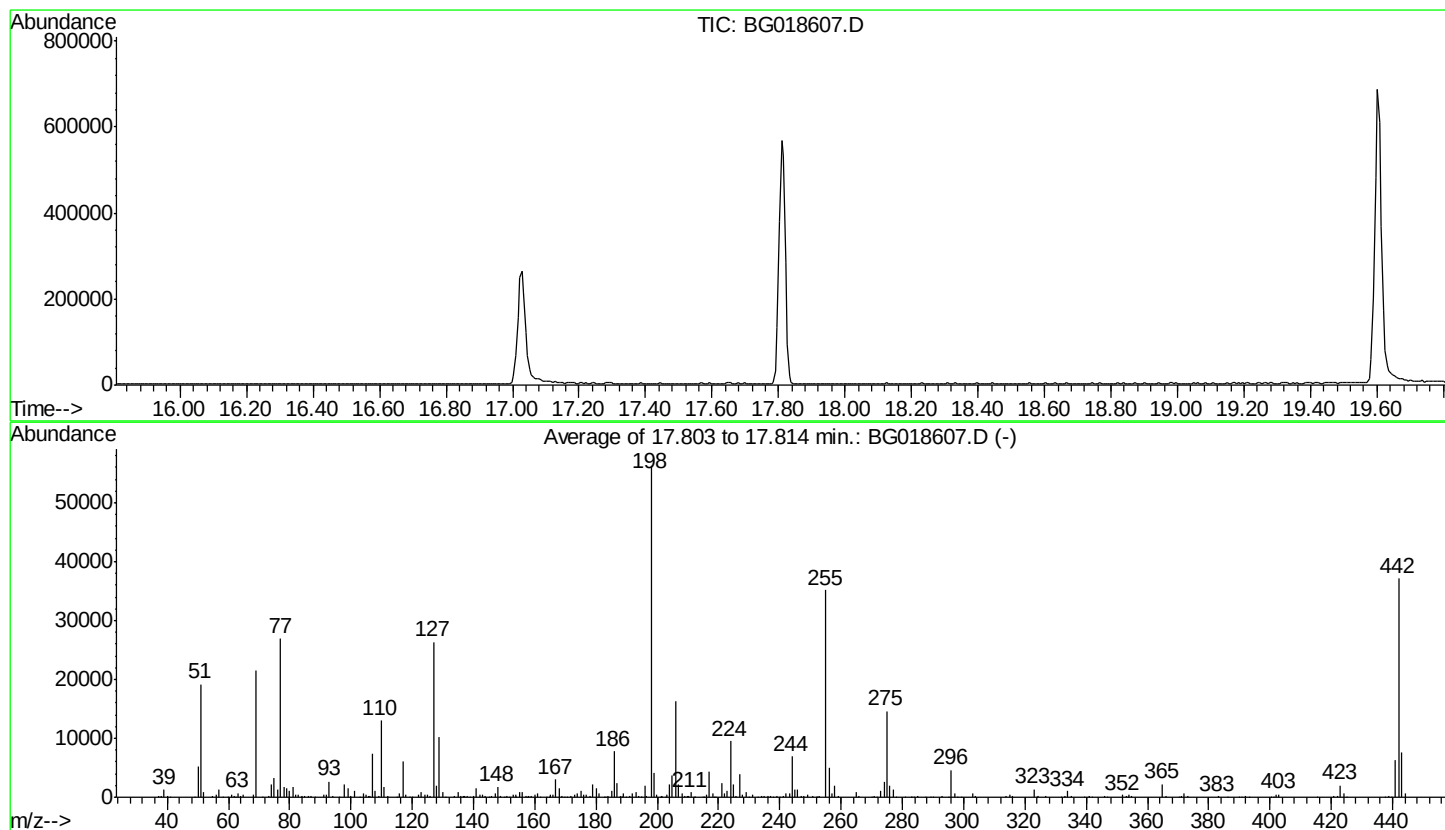

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2541

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 34.1      | 19189   | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 423     | PASS             |
| 69          | 198          | 0.00         | 100          | 38.1      | 21437   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 46.8      | 26333   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 56322   | PASS             |
| 199         | 198          | 5            | 9            | 7.5       | 4215    | PASS             |
| 275         | 198          | 10           | 60           | 26.0      | 14666   | PASS             |
| 365         | 198          | 1            | 100          | 4.0       | 2228    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.8      | 6245    | PASS             |
| 442         | 198          | 50           | 100          | 65.9      | 37114   | PASS             |
| 443         | 442          | 15           | 24           | 20.3      | 7529    | PASS             |