
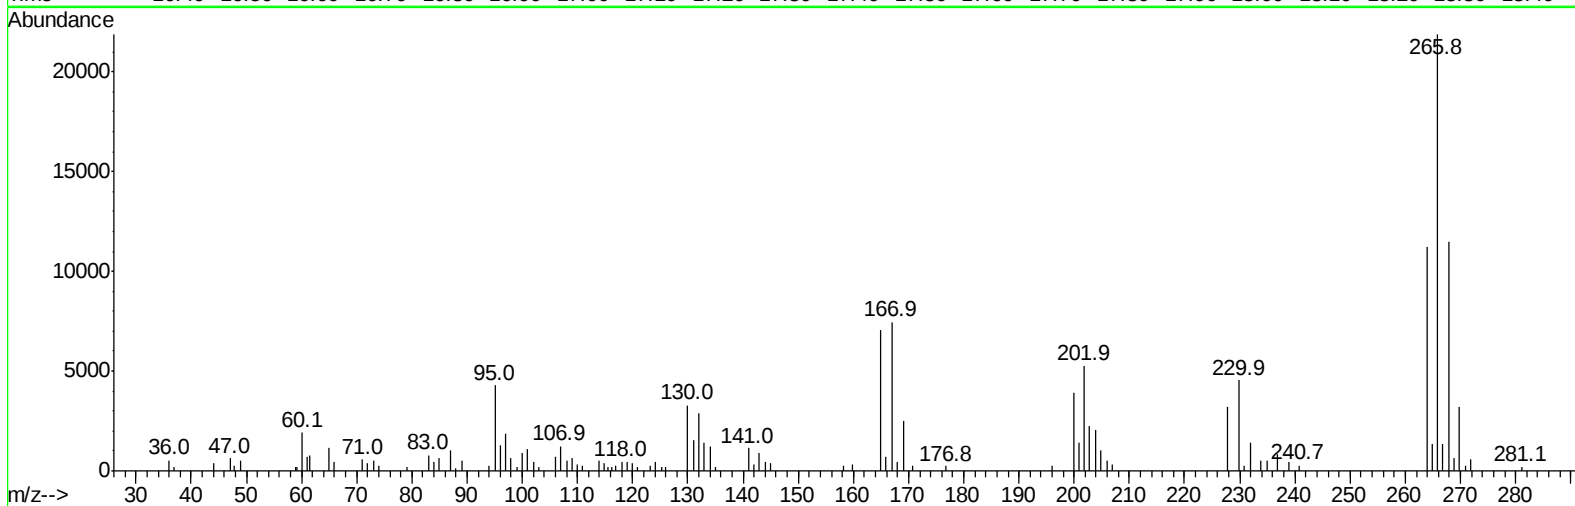


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091117\
Data File : BG028651.D
Acq On : 11 Sep 2017 21:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 07:25:32 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG090717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 07 18:39:50 2017
Response via : Initial Calibration

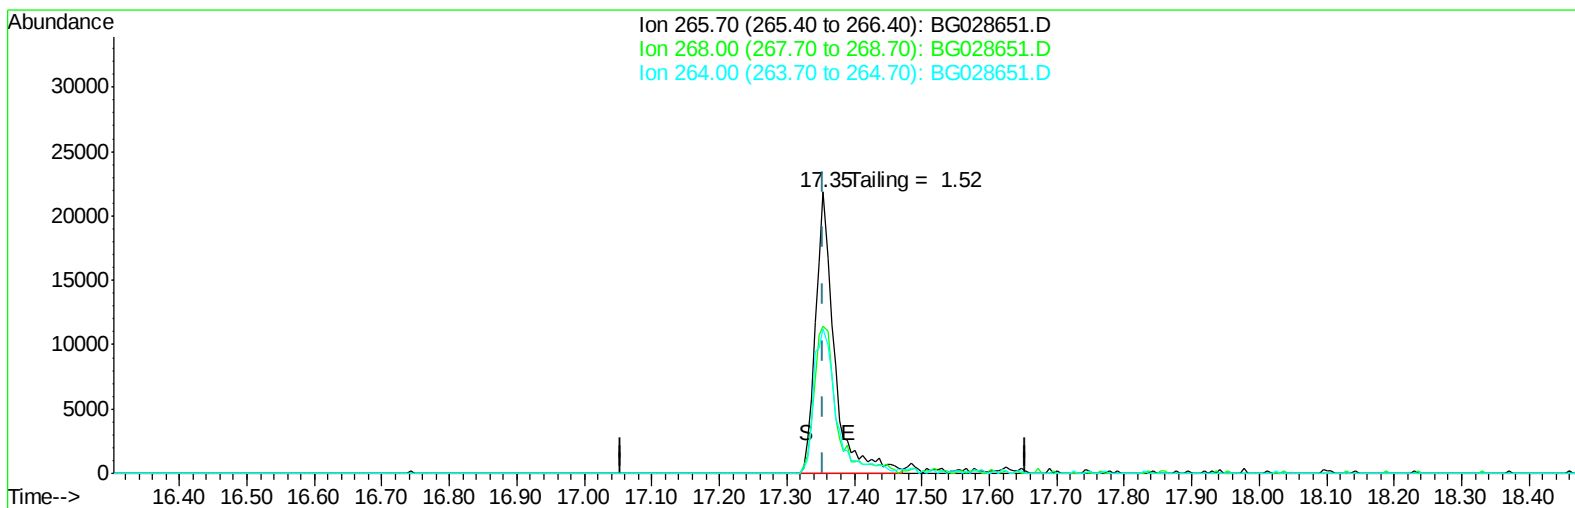

TIC: BG028651.D

(69) Pentachlorophenol (C)



17.354min (+0.000) 86726.64ng

response 41530

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	52.44
264.00	62.60	51.33
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091117\
Data File : BG028651.D
Acq On : 11 Sep 2017 21:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 07:25:32 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG090717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 07 18:39:50 2017
Response via : Initial Calibration

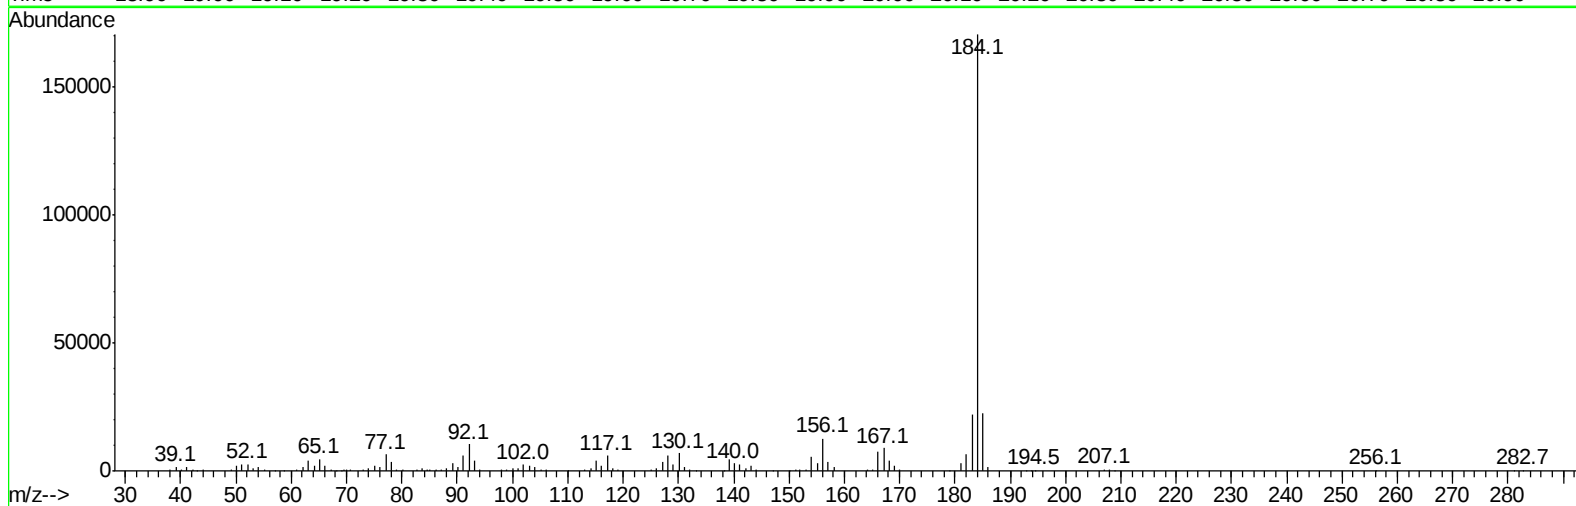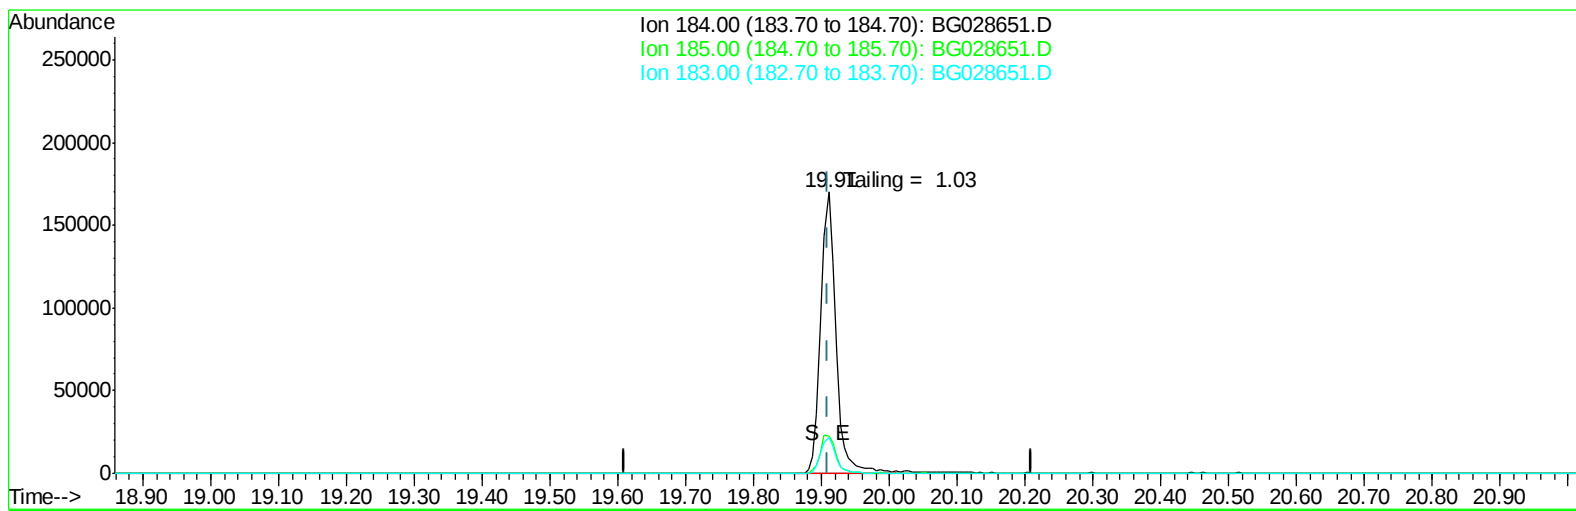

TIC: BG028651.D

(76) Benzidine

19.910min (+0.000) 213507.32ng

response 260253

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.31
183.00	13.80	12.81
0.00	0.00	0.00