


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG091117\
 Data File : BG028651.D
 Acq On : 11 Sep 2017 21:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG090717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 07 18:39:50 2017

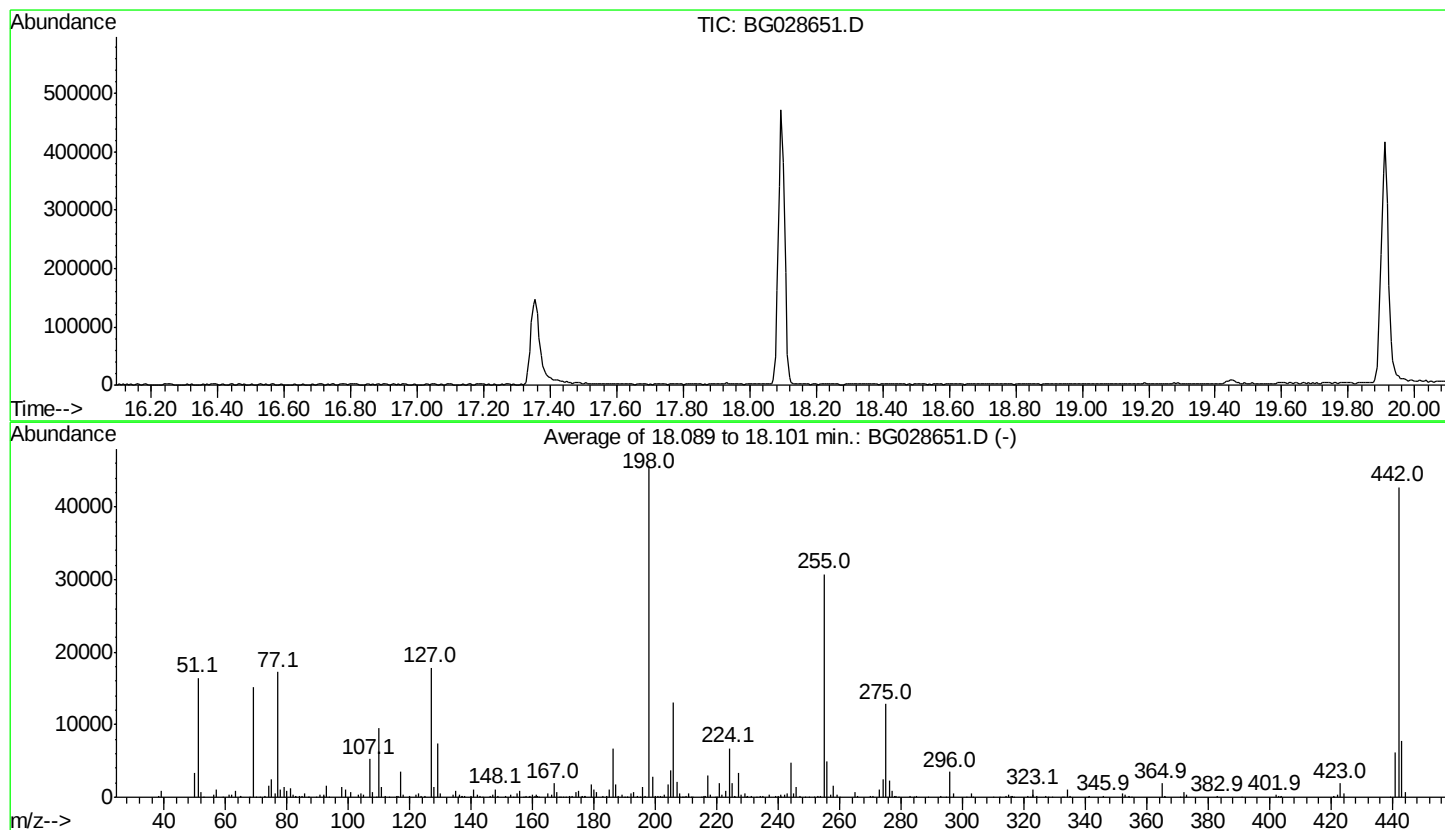

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	16403	PASS
68	69	0.00	2	0.5	81	PASS
69	198	0.00	100	33.4	15238	PASS
70	69	0.00	2	0.5	76	PASS
127	198	10	80	39.0	17833	PASS
197	198	0.00	2	0.4	180	PASS
198	198	100	100	100.0	45682	PASS
199	198	5	9	6.1	2776	PASS
275	198	10	60	28.0	12793	PASS
365	198	1	100	4.1	1872	PASS
441	442	0.01	24	14.5	6173	PASS
442	198	50	100	93.5	42693	PASS
443	442	15	24	18.3	7831	PASS