
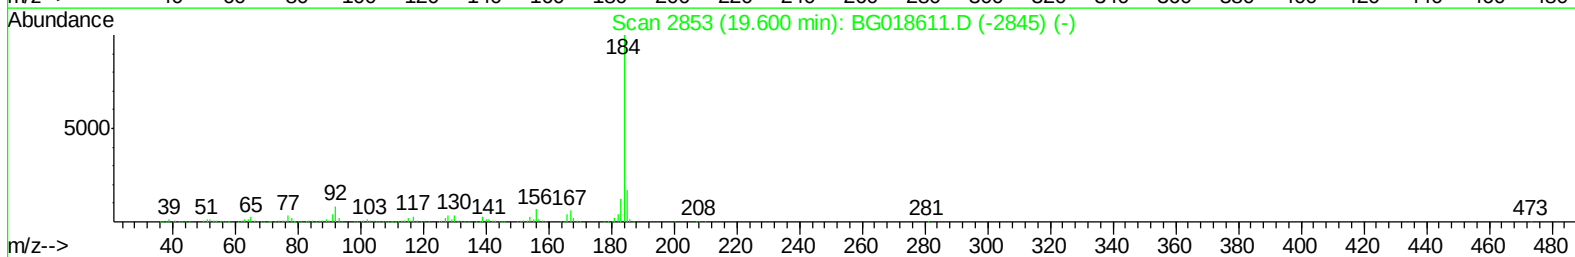
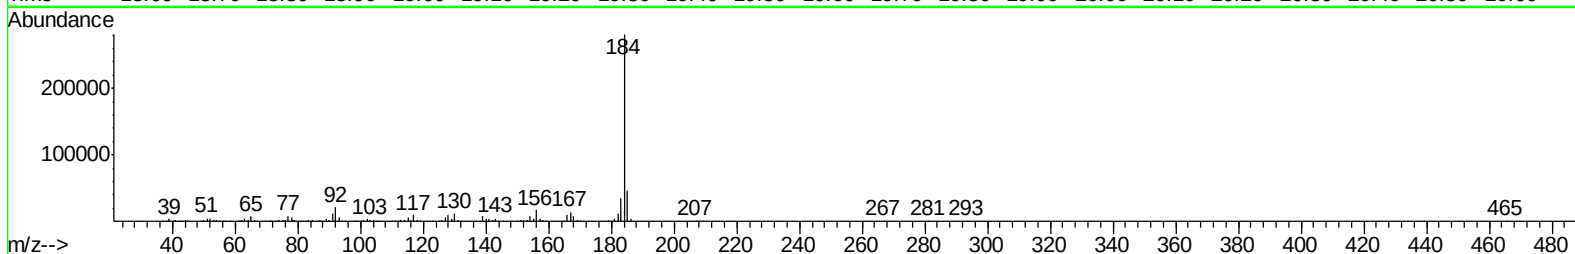


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091215\
 Data File : BG018632.D
 Acq On : 11 Sep 2015 10:25
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 11 17:01:12 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 11 10:44:16 2015
 Response via : Initial Calibration

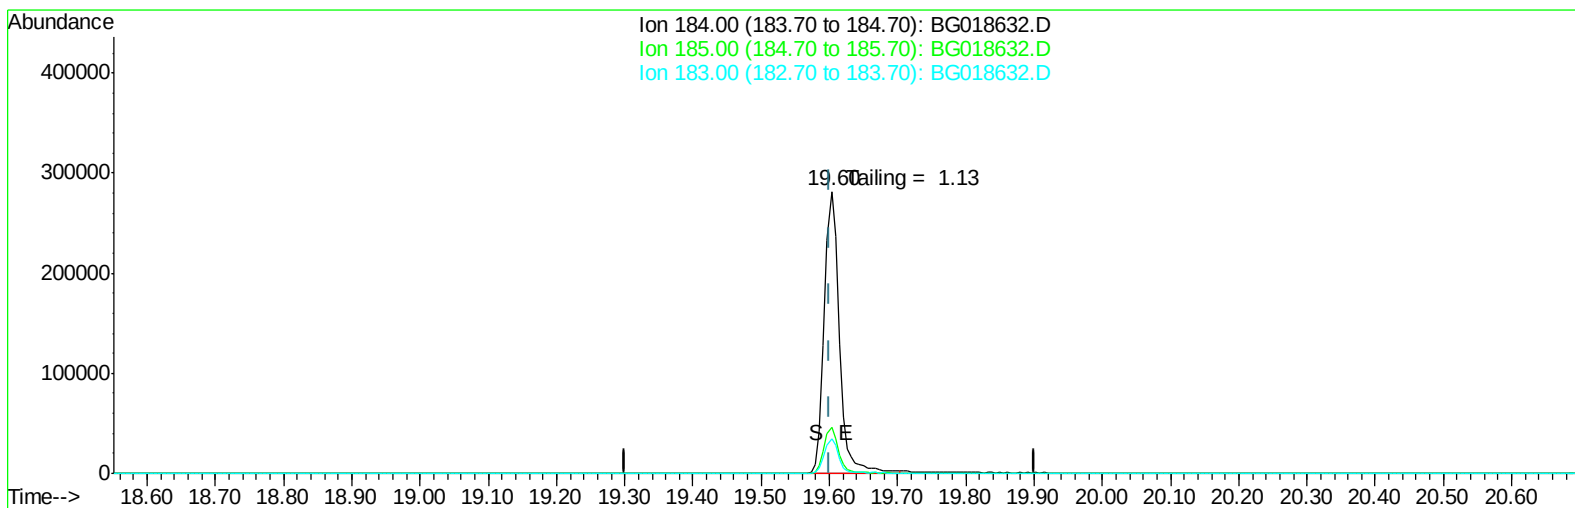

TIC: BG018632.D

(76) Benzidine




19.603min (+0.002) 254314.96ng

response 427677

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	16.58
183.00	12.60	12.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091215\
Data File : BG018632.D
Acq On : 11 Sep 2015 10:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 11 17:01:12 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 11 10:44:16 2015
Response via : Initial Calibration

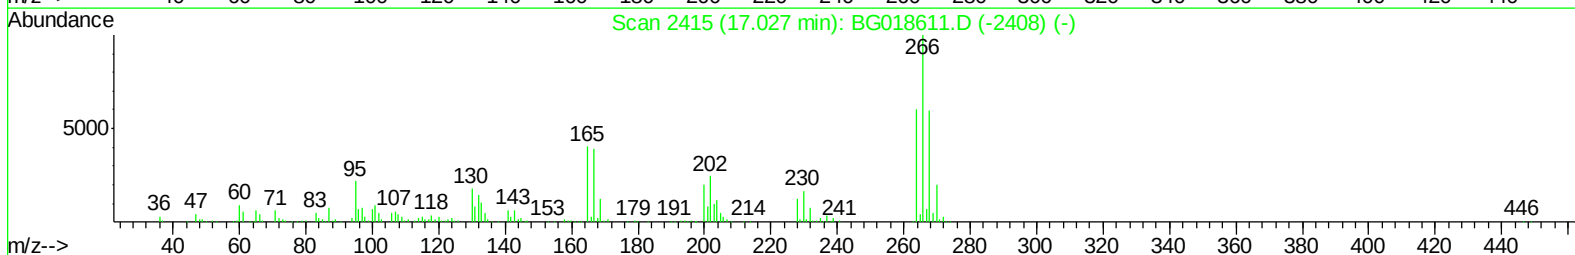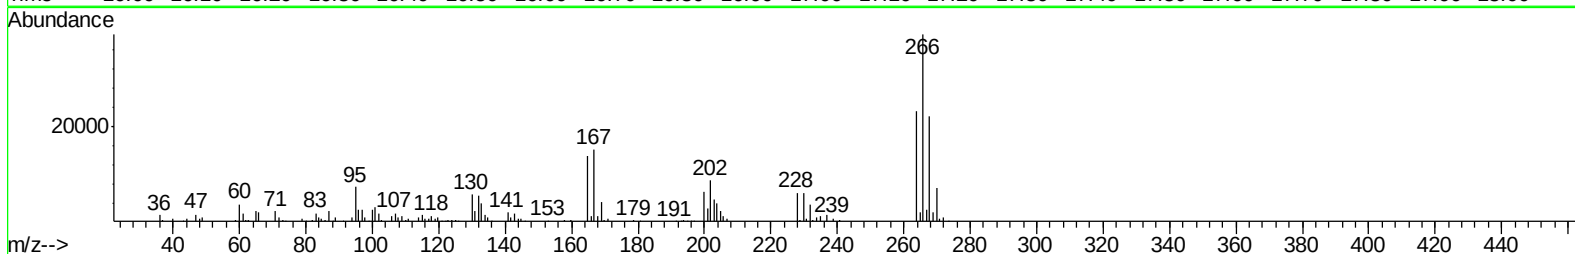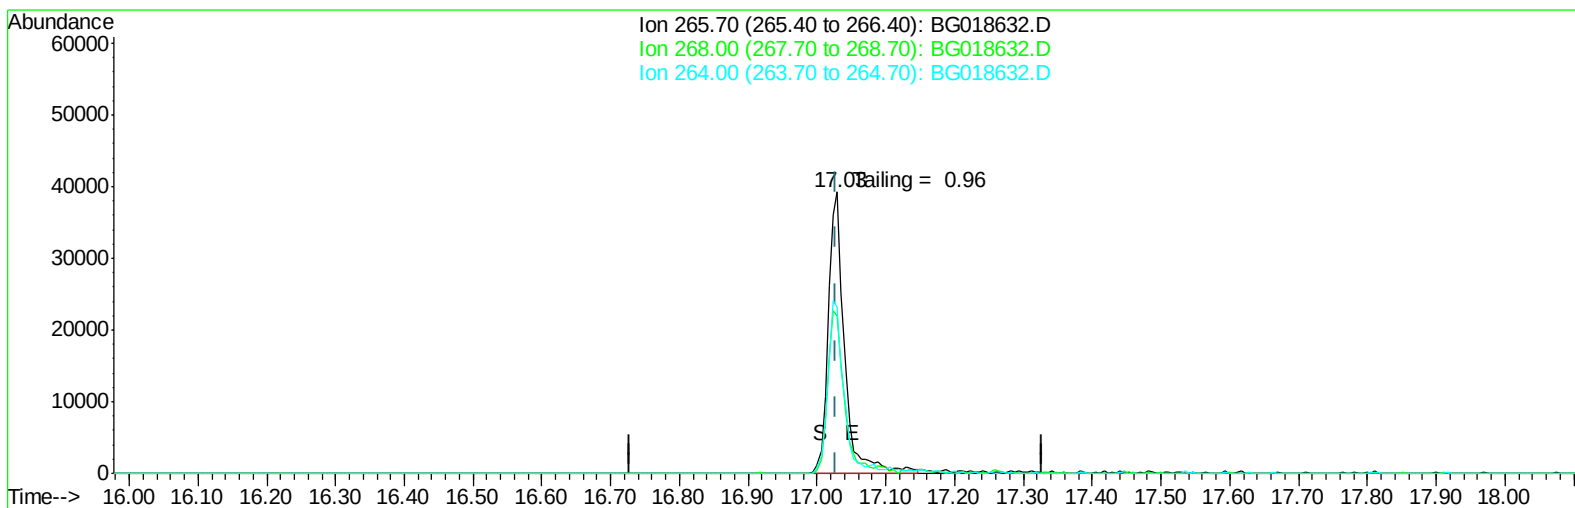

TIC: BG018632.D

(69) Pentachlorophenol (C)

17.029min (+0.002) 122652.81ng

response 63524

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	61.13
264.00	60.10	58.95
0.00	0.00	0.00