
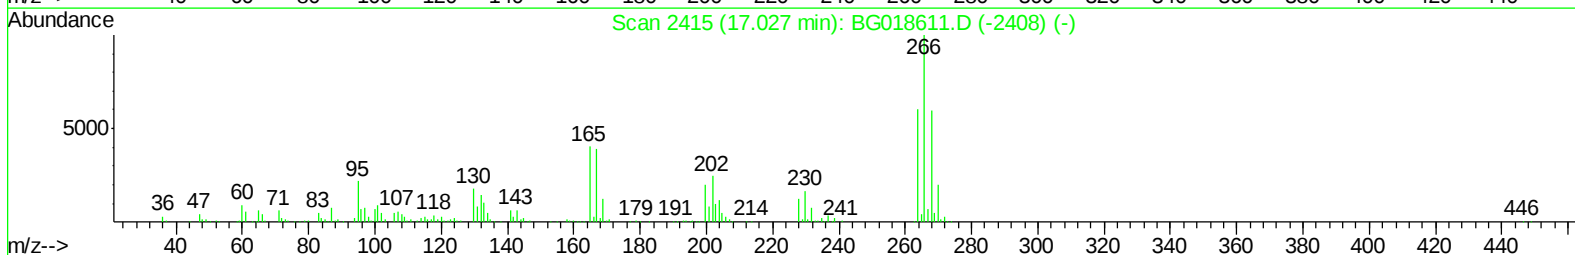
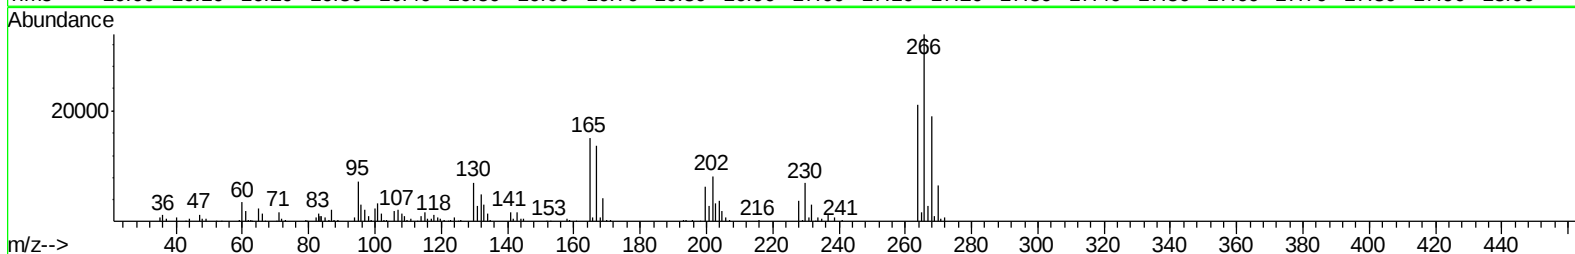


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091215\
Data File : BG018648.D
Acq On : 11 Sep 2015 20:43
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 12 02:35:29 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 11 10:44:16 2015
Response via : Initial Calibration

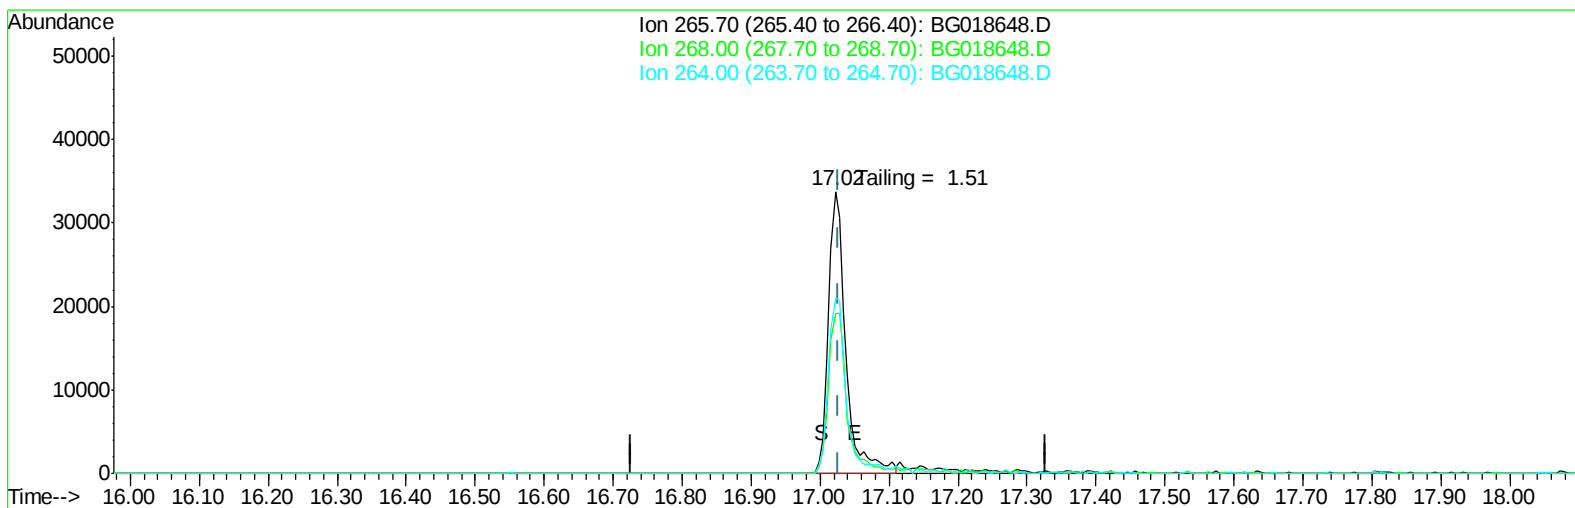

TIC: BG018648.D

(69) Pentachlorophenol (C)




17.022min (-0.006) 139120.66ng

response 57832

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	56.62
264.00	60.10	62.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091215\
Data File : BG018648.D
Acq On : 11 Sep 2015 20:43
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 12 02:35:29 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 11 10:44:16 2015
Response via : Initial Calibration

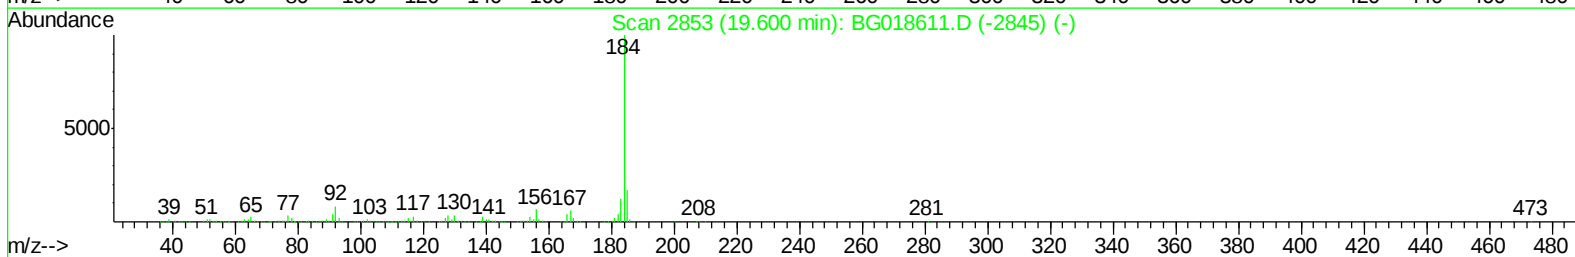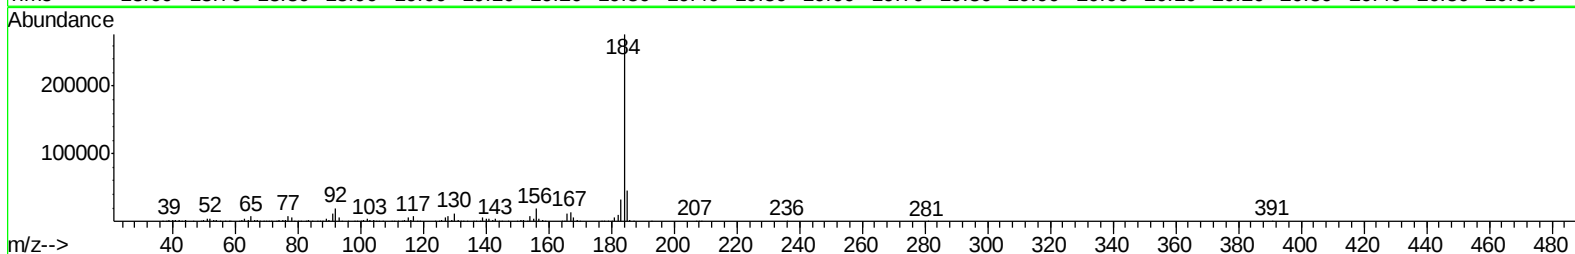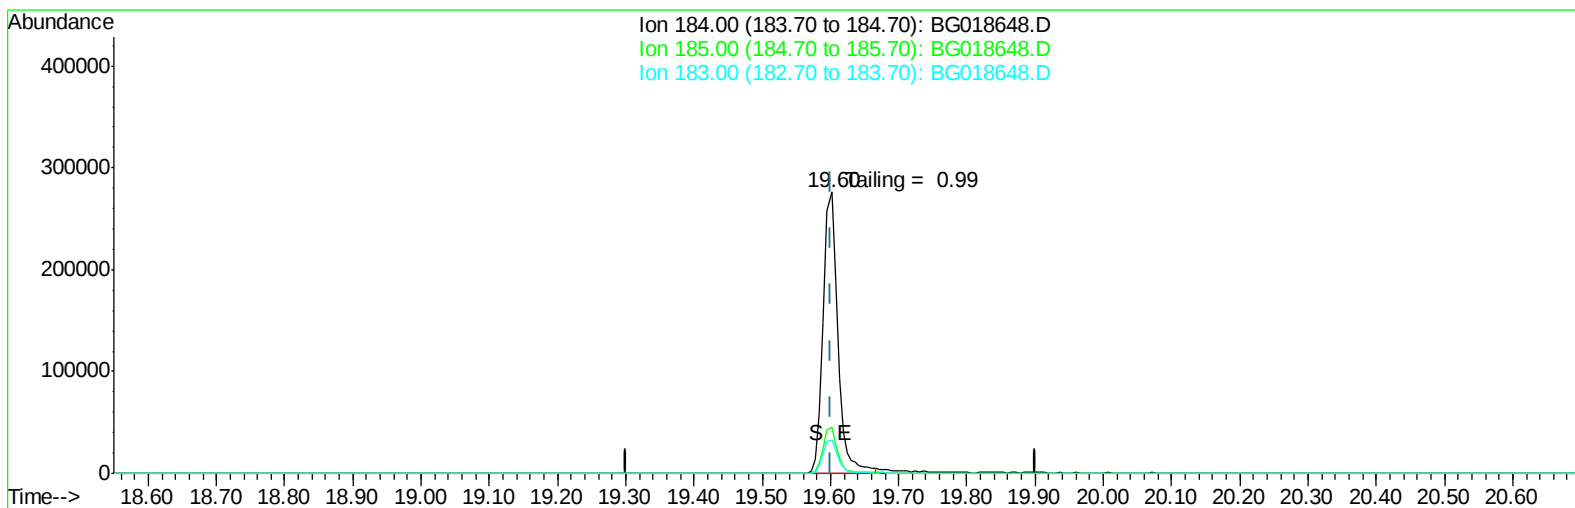

TIC: BG018648.D

(76) Benzidine

19.601min (+0.000) 249688.74ng

response 412399

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	16.42
183.00	12.60	11.79
0.00	0.00	0.00