


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091215\
 Data File : BG018632.D
 Acq On : 11 Sep 2015 10:25
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 11 10:44:16 2015

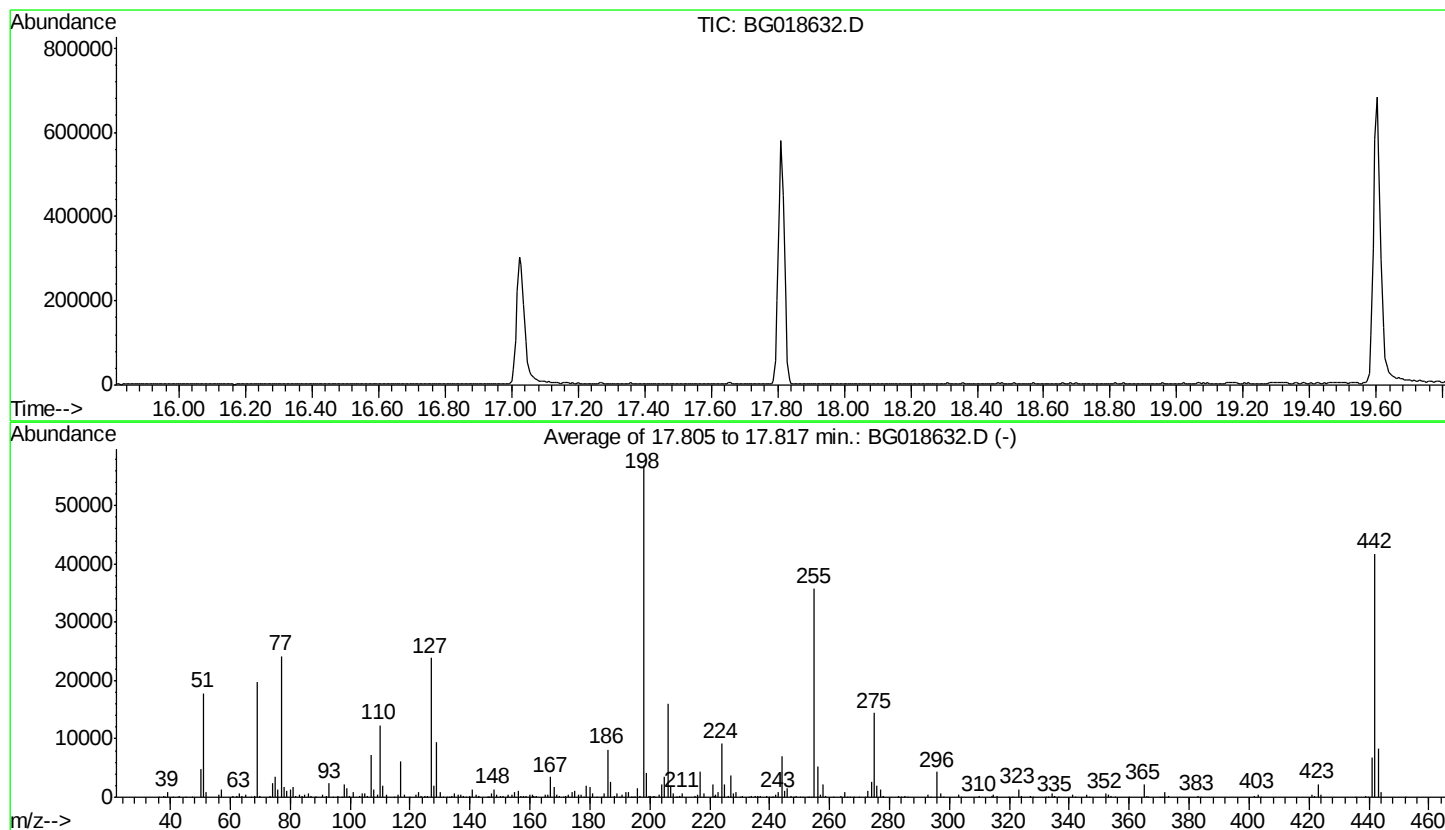

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	17822	PASS
68	69	0.00	2	1.2	243	PASS
69	198	0.00	100	34.9	19861	PASS
70	69	0.00	2	1.1	218	PASS
127	198	10	80	41.9	23826	PASS
197	198	0.00	2	0.2	139	PASS
198	198	100	100	100.0	56866	PASS
199	198	5	9	7.3	4125	PASS
275	198	10	60	25.4	14435	PASS
365	198	1	100	3.7	2131	PASS
441	442	0.01	24	16.3	6823	PASS
442	198	50	100	73.5	41794	PASS
443	442	15	24	20.0	8349	PASS