


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091215\
 Data File : BG018648.D
 Acq On : 11 Sep 2015 20:43
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 11 10:44:16 2015

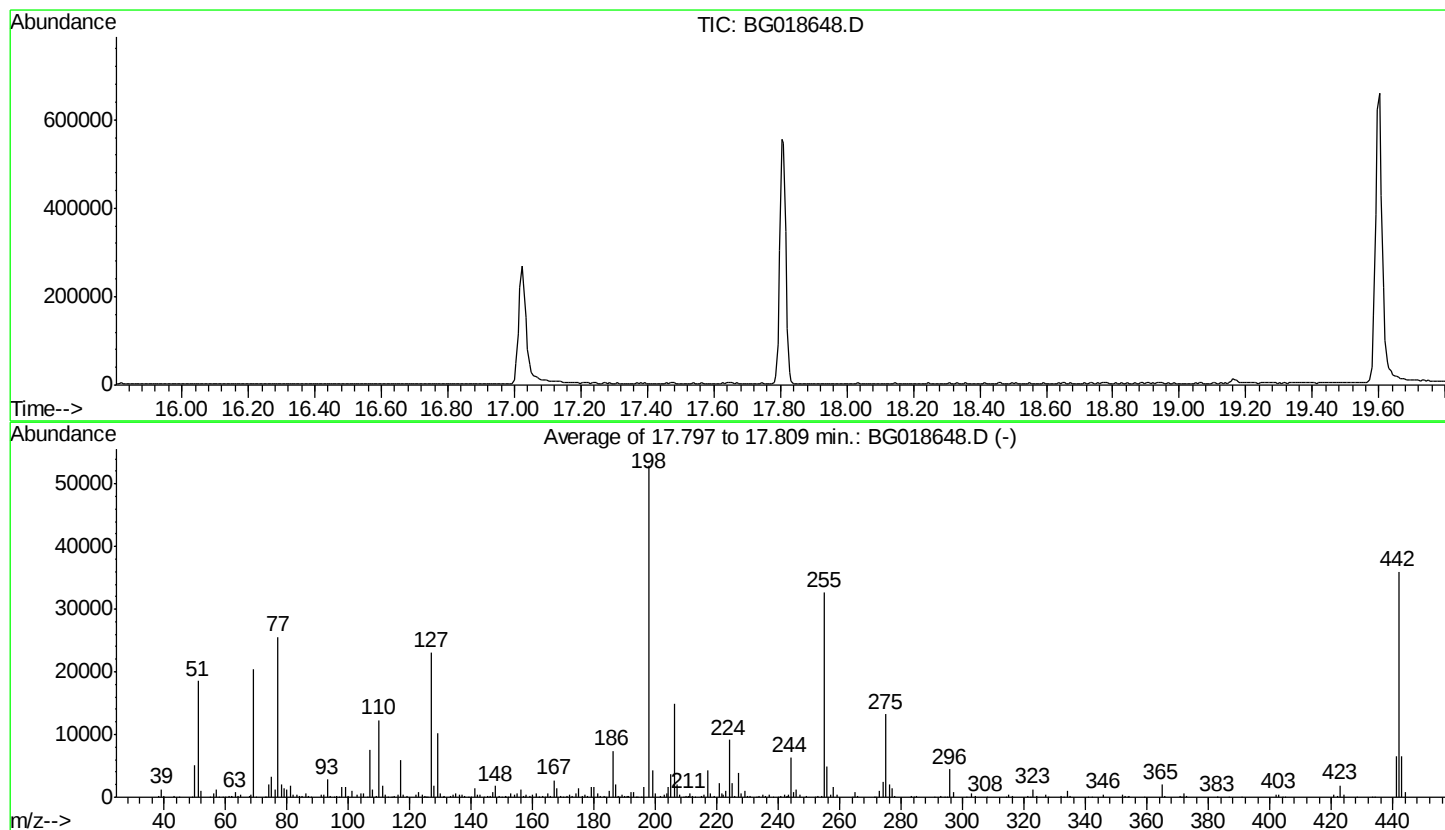

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	18572	PASS
68	69	0.00	2	1.5	316	PASS
69	198	0.00	100	38.6	20428	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	43.6	23059	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52893	PASS
199	198	5	9	7.9	4197	PASS
275	198	10	60	24.9	13189	PASS
365	198	1	100	3.8	2016	PASS
441	442	0.01	24	18.5	6639	PASS
442	198	50	100	68.0	35954	PASS
443	442	15	24	18.1	6524	PASS