



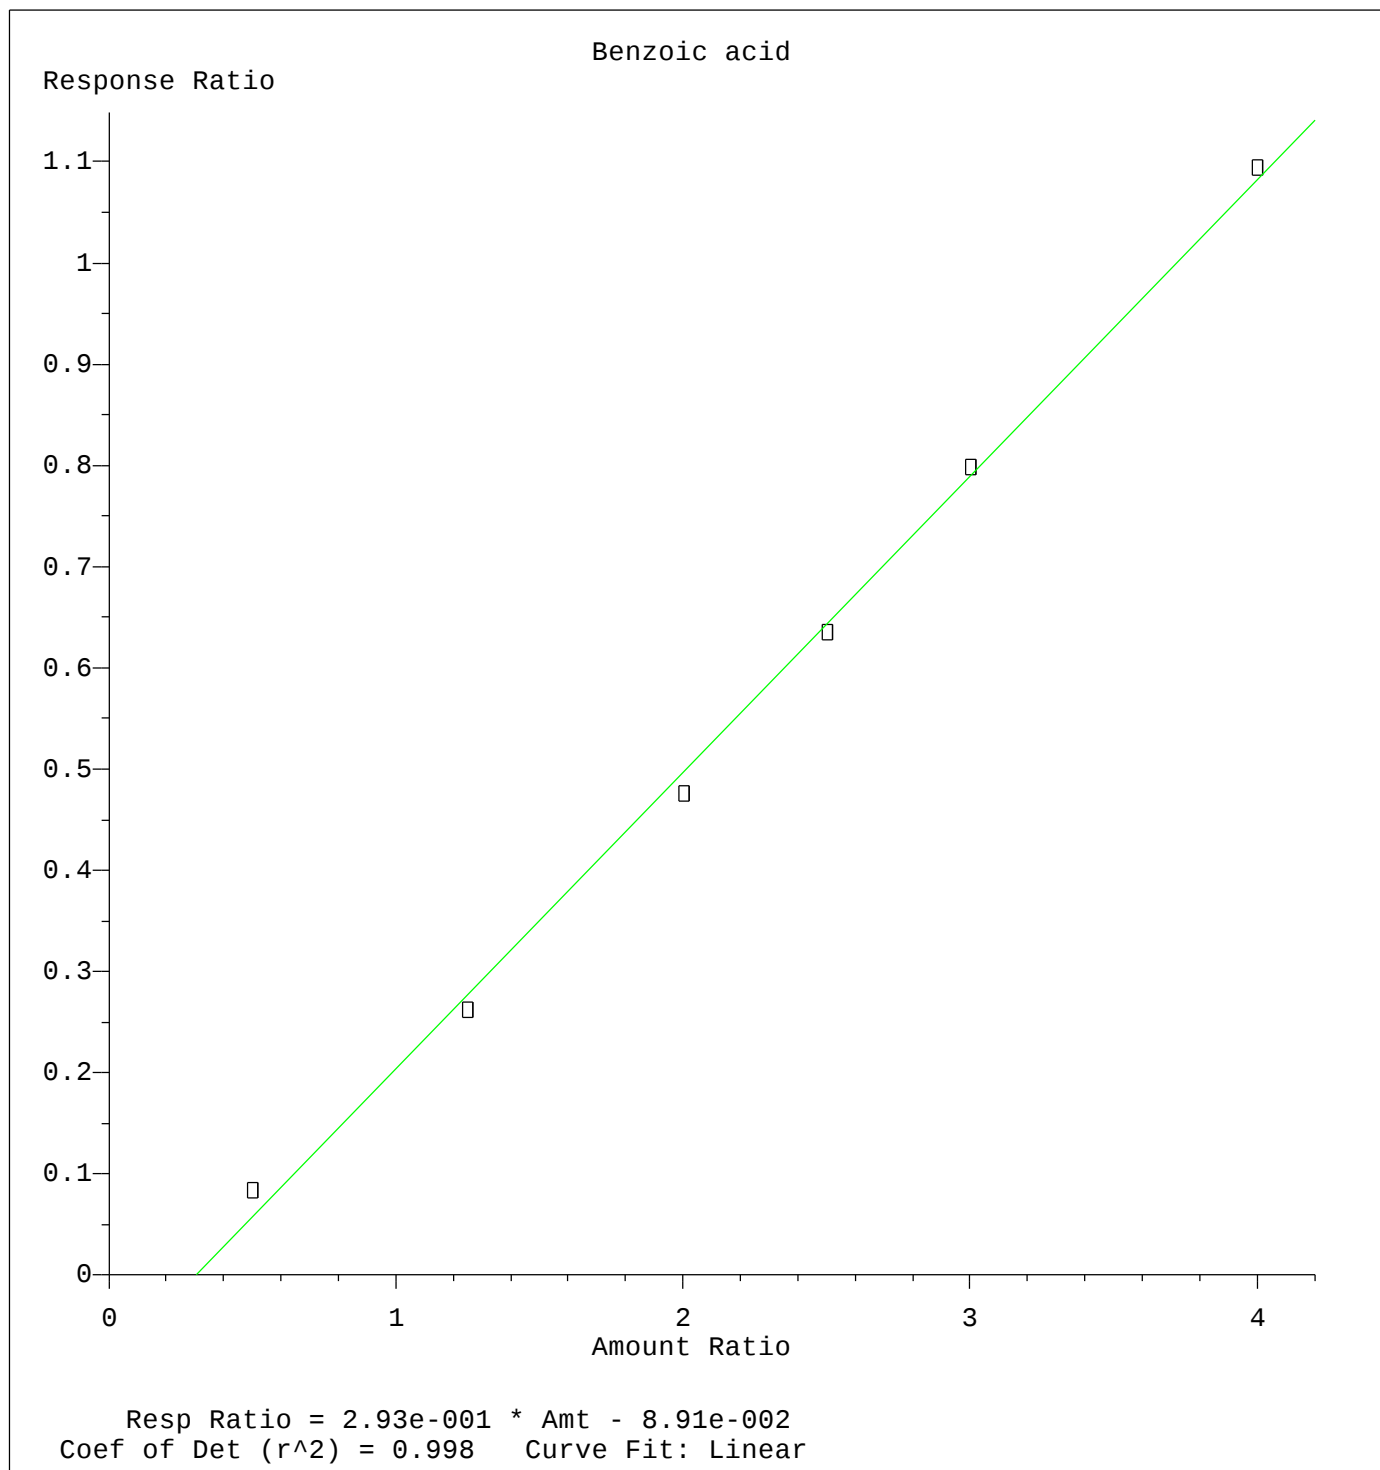

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
Calibration Table Last Updated: Tue Sep 12 16:57:11 2017

Hexachlorocyclopentadiene

Response Ratio

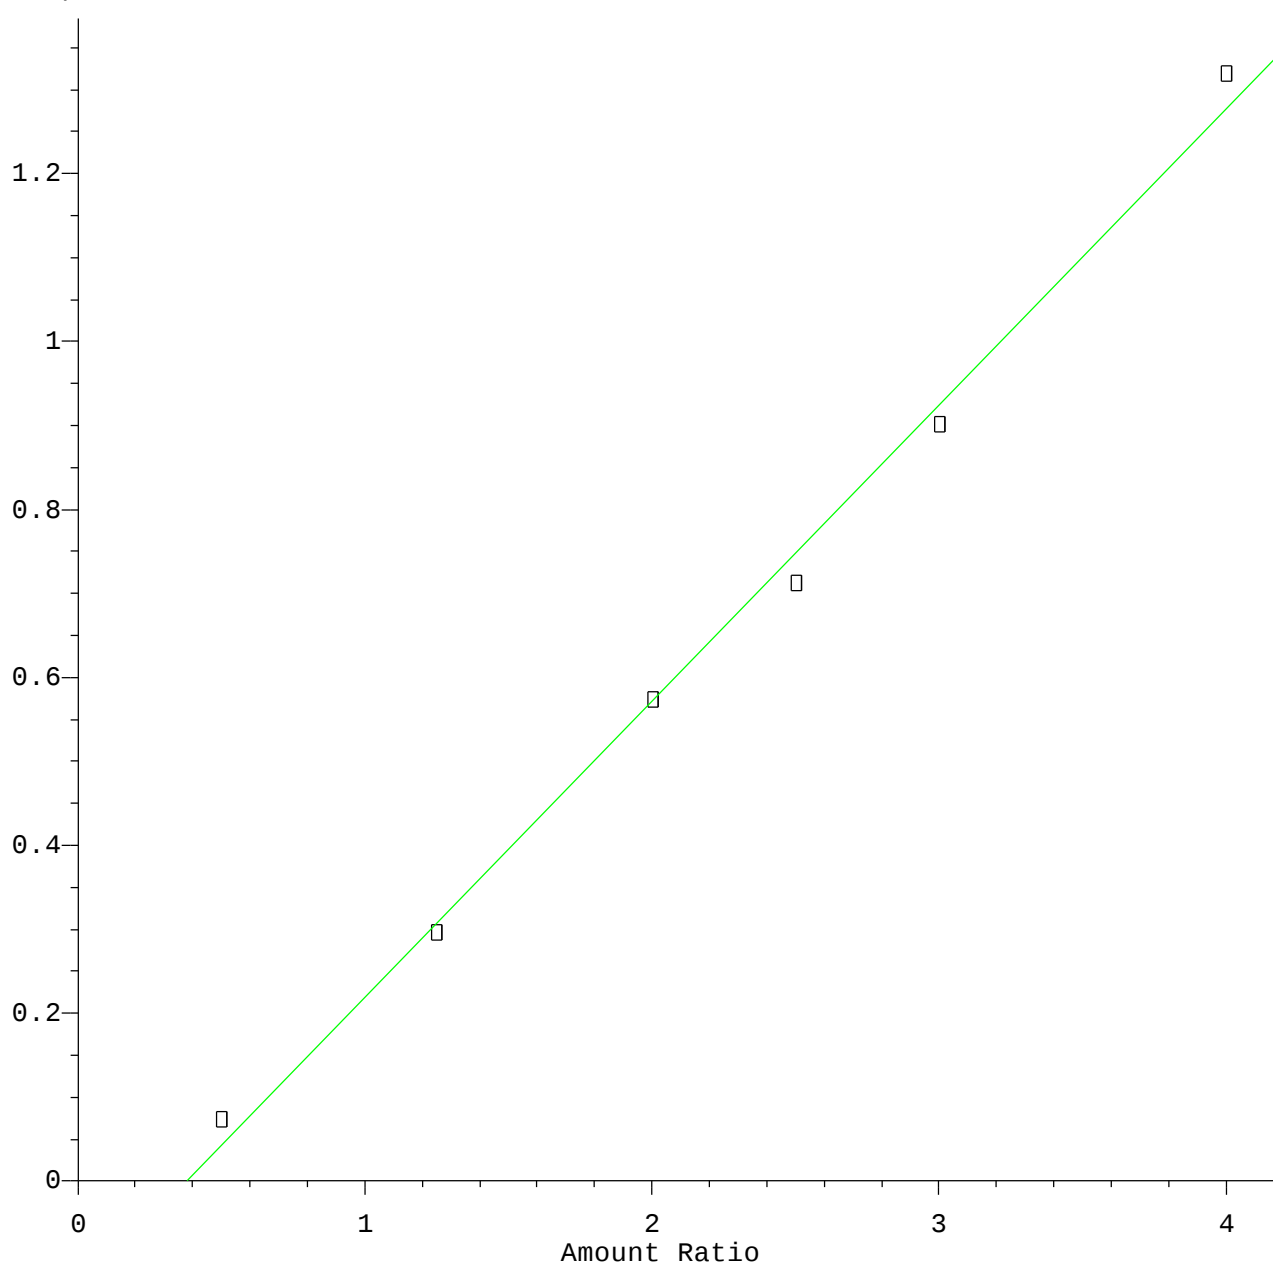


Resp Ratio = $3.53 \times 10^{-1} \times \text{Amt} - 1.34 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
Calibration Table Last Updated: Tue Sep 12 16:57:11 2017

2,4-Dinitrophenol

Response Ratio

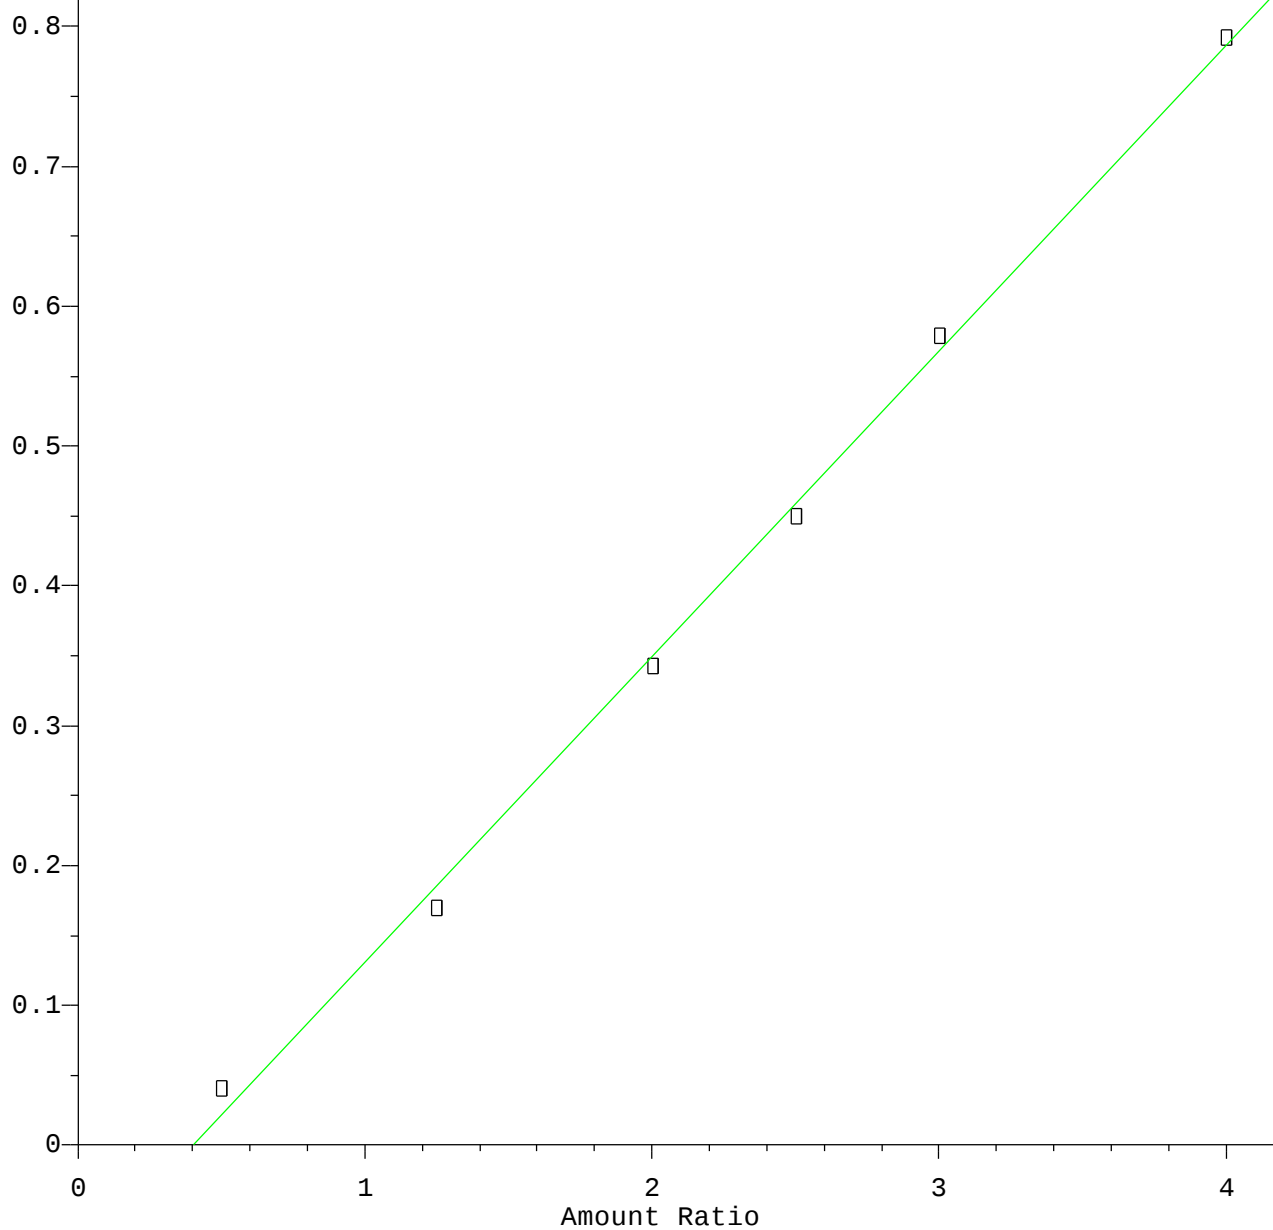

Resp Ratio = $2.18 \times 10^{-1} \times \text{Amt} - 8.74 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
Calibration Table Last Updated: Tue Sep 12 16:57:11 2017