
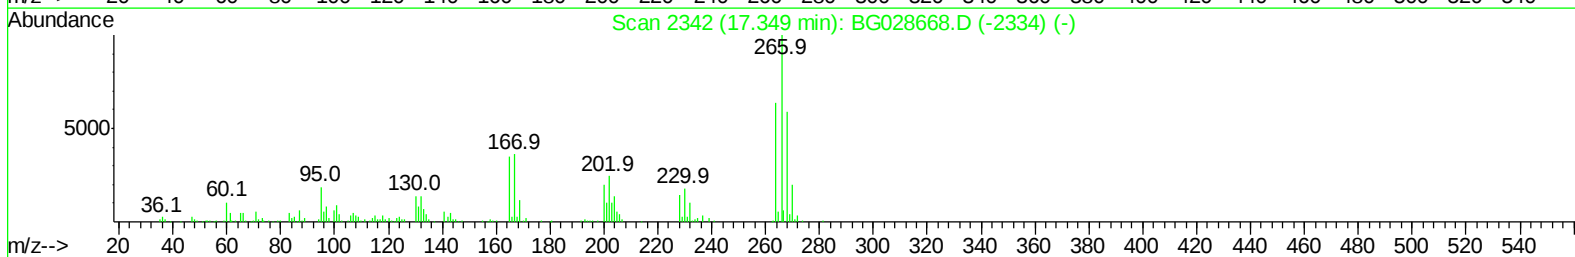
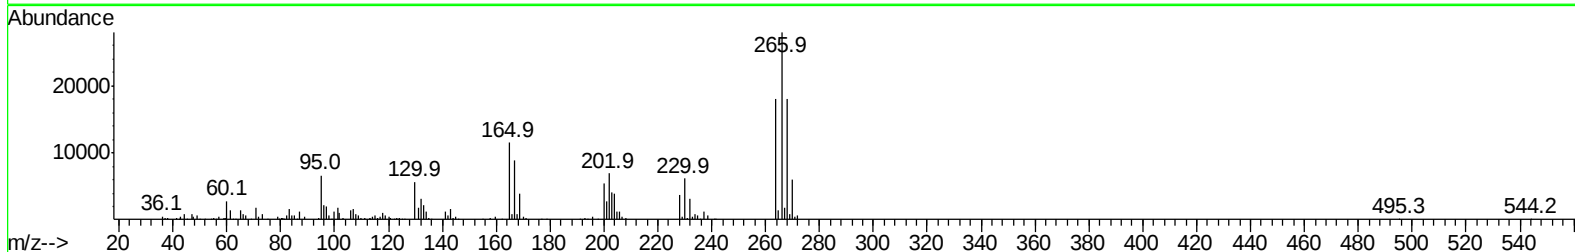


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091217\
Data File : BG028664.D
Acq On : 12 Sep 2017 11:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 17:42:00 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

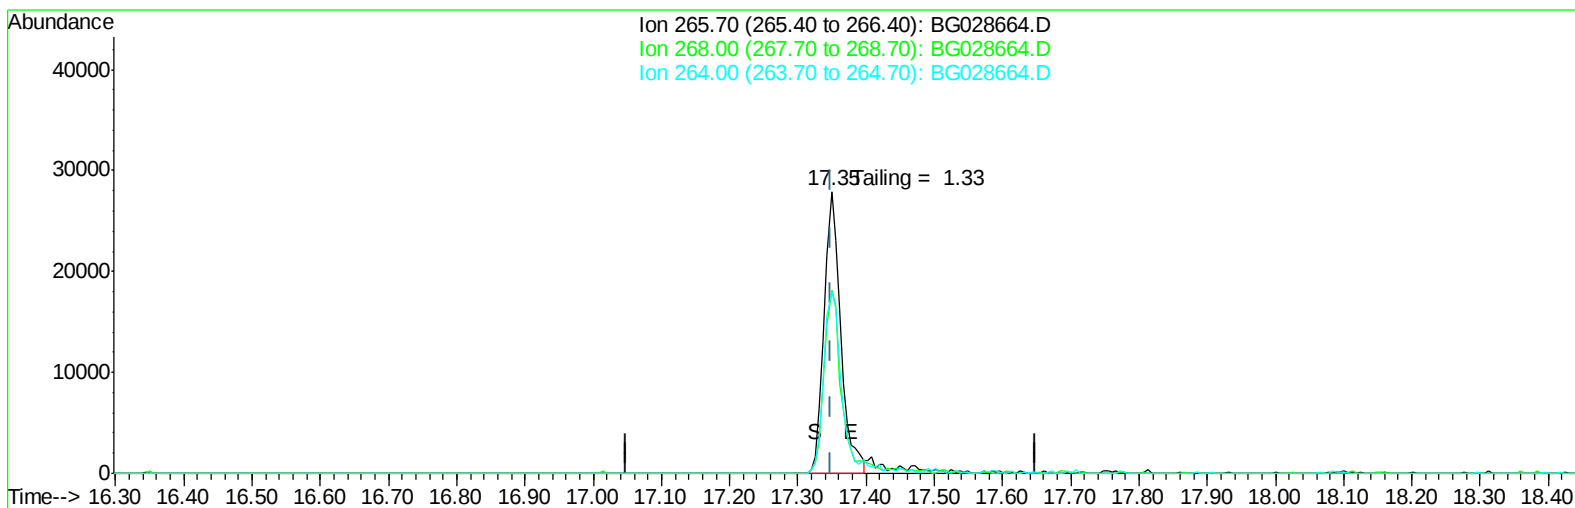

TIC: BG028664.D

(69) Pentachlorophenol (C)




17.349min (+0.000) 135073.77ng

response 49157

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	64.87
264.00	62.60	64.73
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091217\
 Data File : BG028664.D
 Acq On : 12 Sep 2017 11:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 17:42:00 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration

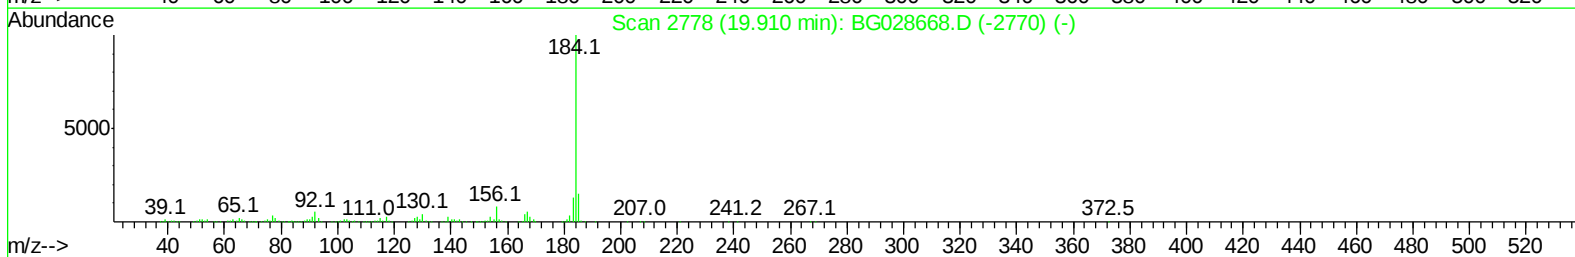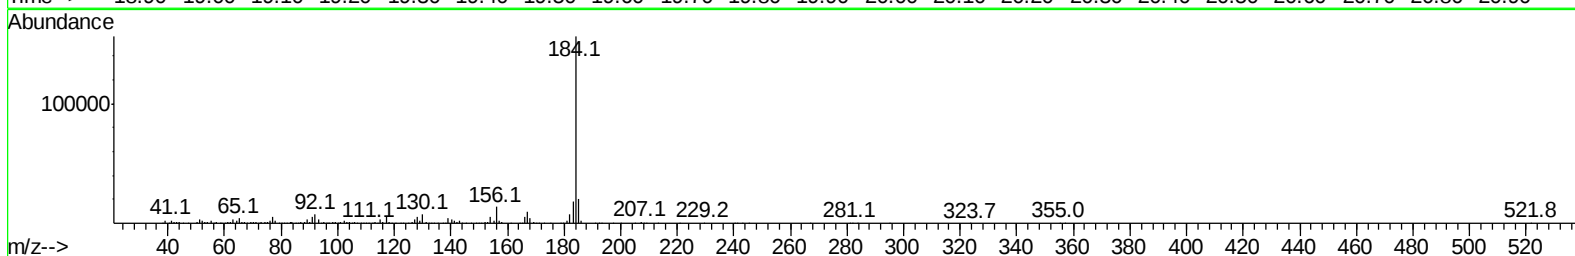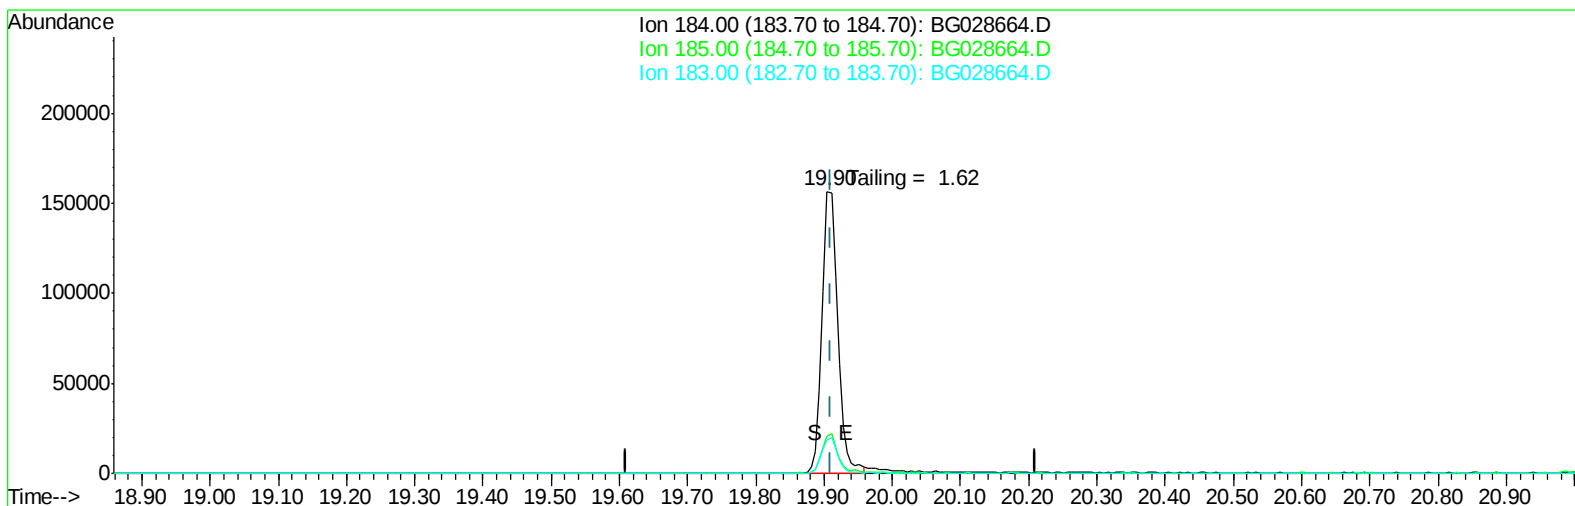

TIC: BG028664.D

(76) Benzidine

19.905min (-0.006) 170203.24ng m

response 247171

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.39
183.00	13.80	12.04
0.00	0.00	0.00