

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091217\
 Data File : BG028676.D
 Acq On : 12 Sep 2017 19:11
 Operator : SJ/JU
 Sample : PB102188BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB102188BL

Quant Time: Sep 13 04:46:07 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	31841	20.00	ng	0.00
21) Naphthalene-d8	11.15	136	122131	20.00	ng	0.00
38) Acenaphthene-d10	14.94	164	88118	20.00	ng	0.00
63) Phenanthrene-d10	17.69	188	265949	20.00	ng	0.00
75) Chrysene-d12	22.03	240	304193	20.00	ng	0.00
86) Perylene-d12	25.53	264	313811	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.90	112	258939	134.19	ng	0.00
7) Phenol-d6	7.49	99	341623	117.58	ng	0.00
23) Nitrobenzene-d5	9.50	82	213855	83.76	ng	0.00
41) 2,4,6-Tribromophenol	16.43	330	212079	145.52	ng	0.00
44) 2-Fluorobiphenyl	13.56	172	558895	84.57	ng	0.00
78) Terphenyl-d14	20.28	244	1128759	79.13	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091217\
Data File : BG028676.D
Acq On : 12 Sep 2017 19:11
Operator : SJ/JU
Sample : PB102188BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB102188BL

Quant Time: Sep 13 04:46:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

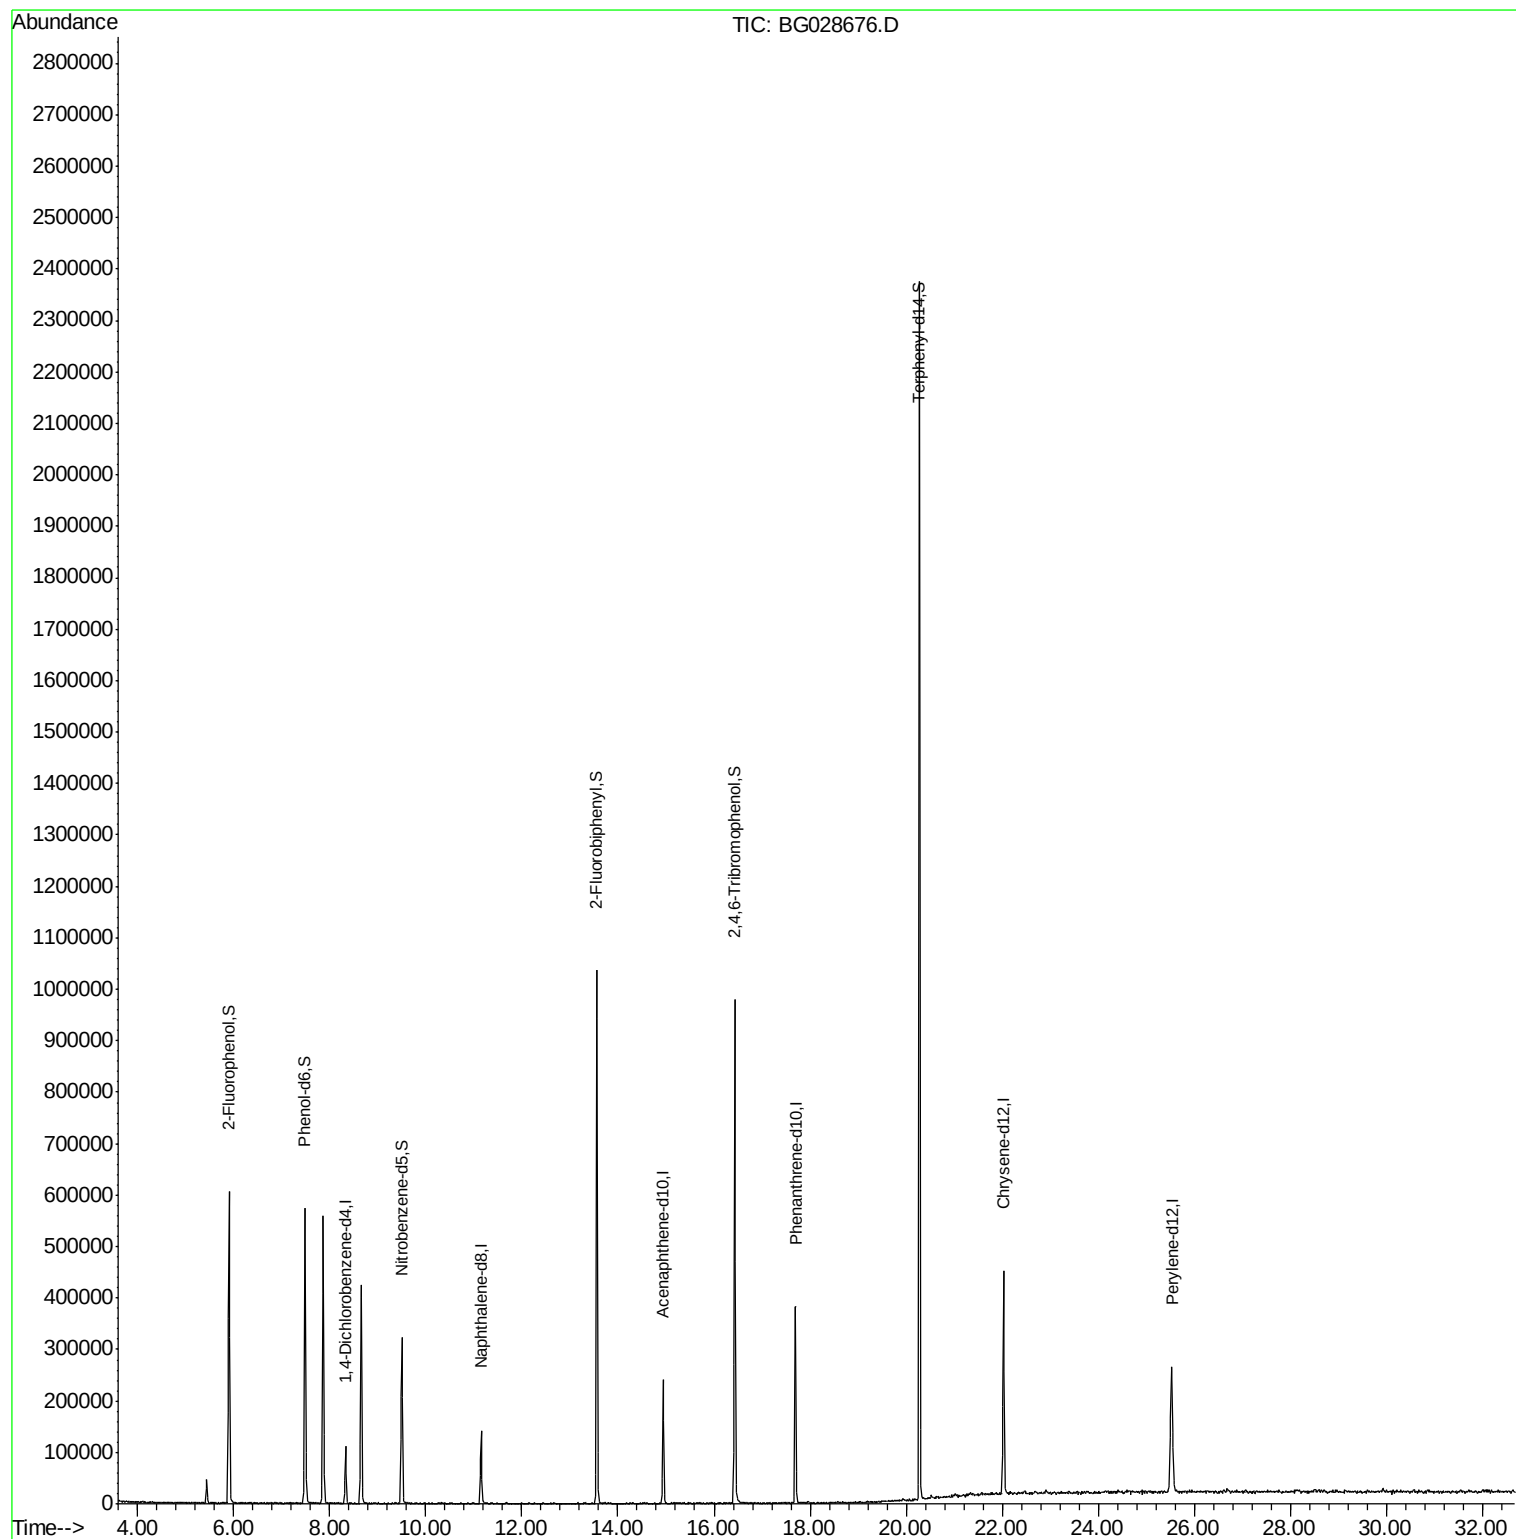

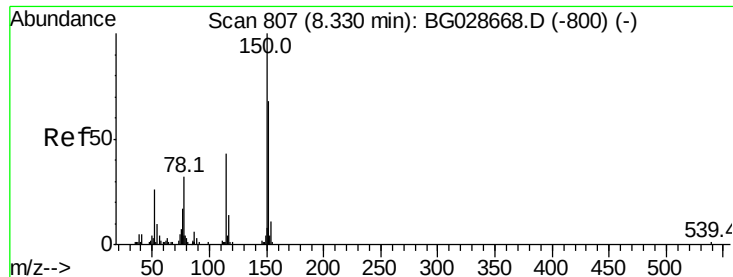

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.33 min Scan# 806

Delta R.T. -0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11

Instrument :

BNA_G

ClientSampleId :

PB102188BL


Tot Ion:152 Resp: 31841

Ion Ratio Lower Upper

152 100

150 153.9 114.0 171.0




115 62.1 48.1 72.1

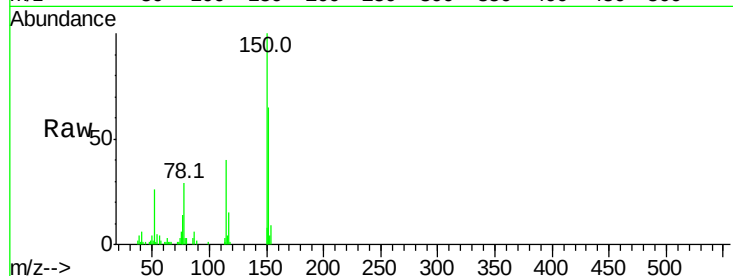

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

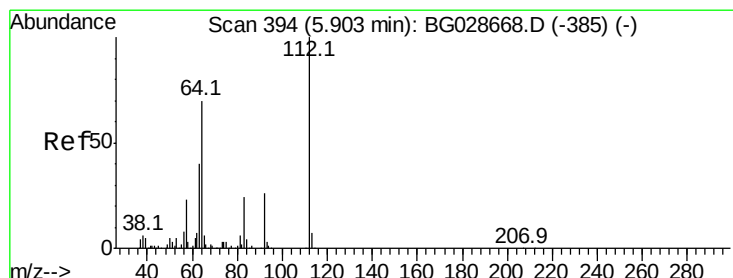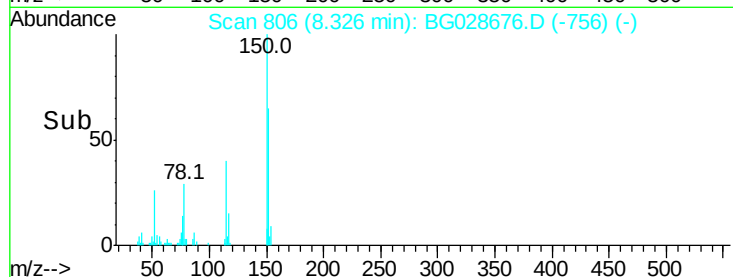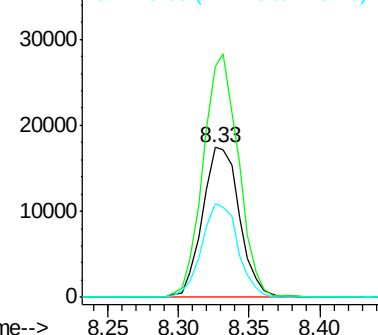

#5

2-Fluorophenol

Concen: 134.186 ng

RT: 5.90 min Scan# 394

Delta R.T. 0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11


Tgt Ion:112 Resp: 258939

Ion Ratio Lower Upper

112 100

64 68.9 61.8 92.6



63 37.1 37.2 55.8#

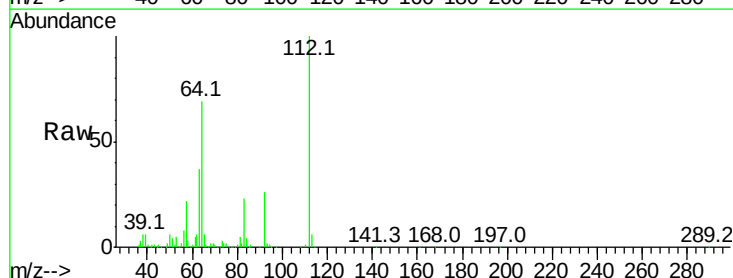


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

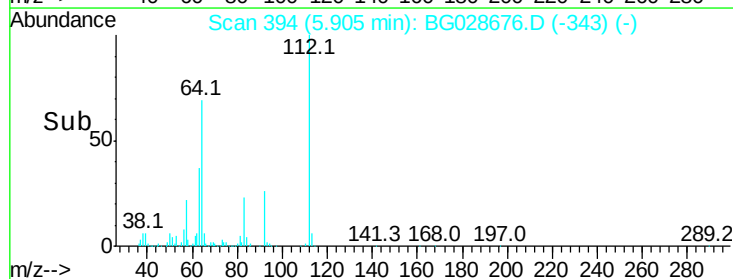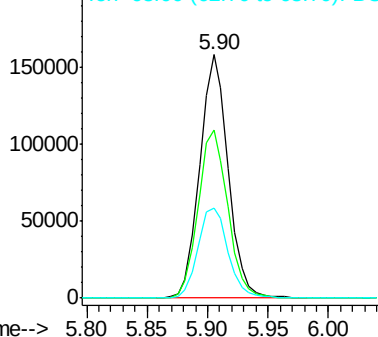

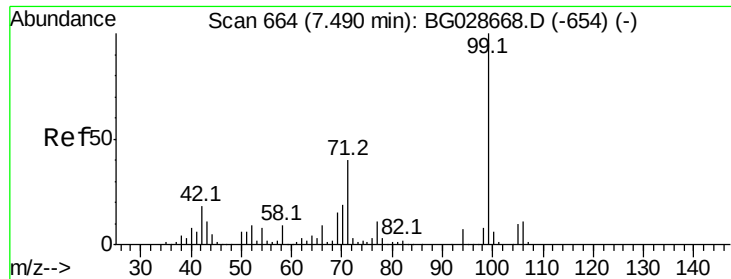

#7

Phenol-d6

Concen: 117.582 ng

RT: 7.49 min Scan# 663

Delta R.T. -0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11

Instrument :

BNA_G

ClientSampleId :

PB102188BL


Tot Ion: 99 Resp: 341623

Ion Ratio Lower Upper




99 100

42 19.1 20.5 30.7#

71 42.3 37.6 56.4

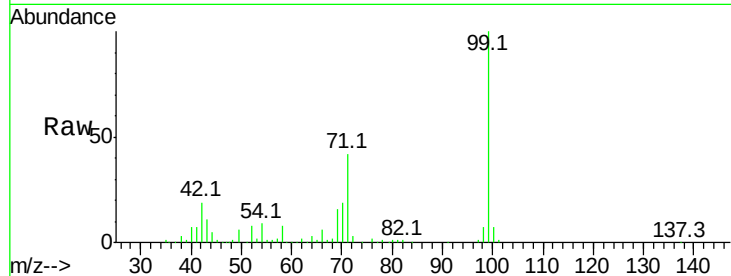

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

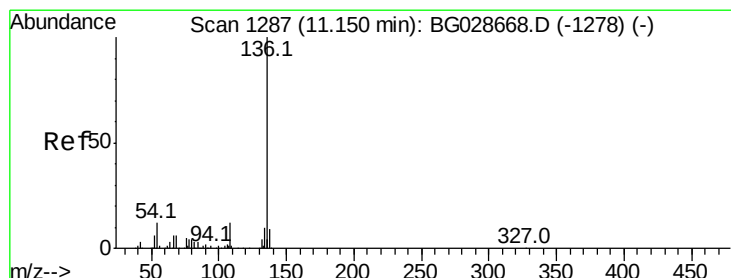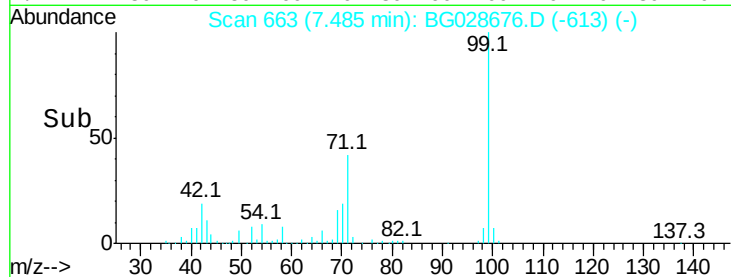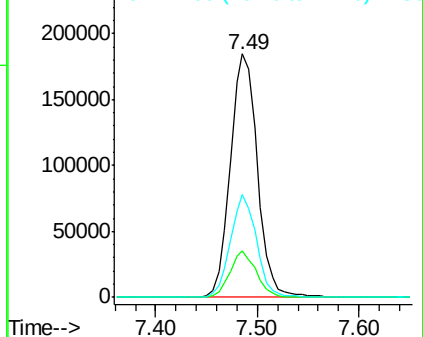

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.15 min Scan# 1287

Delta R.T. 0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11

Tgt Ion: 136 Resp: 122131


Ion Ratio Lower Upper

136 100



137 9.3 8.9 13.3


54 11.1 9.3 13.9

68 4.3 5.1 7.7#

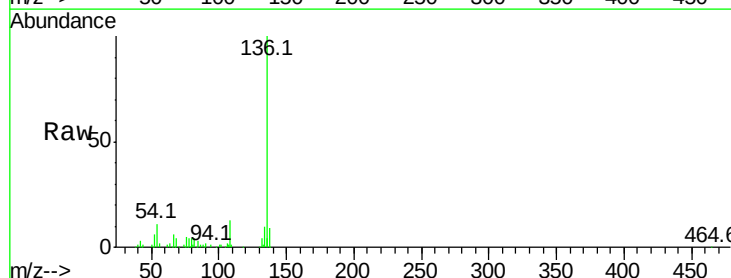

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

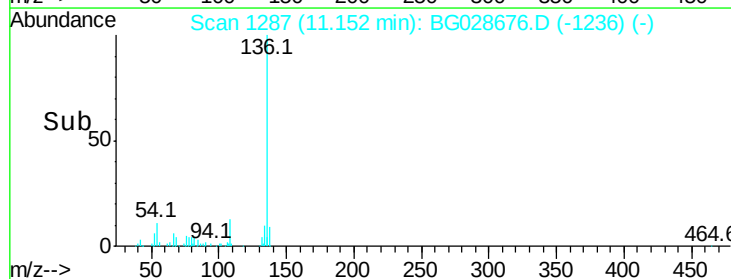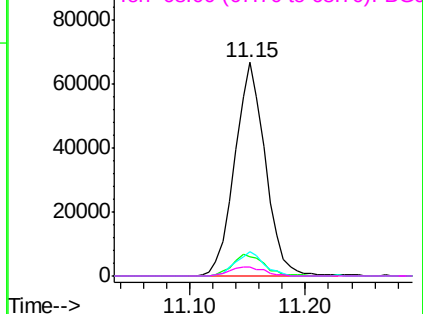

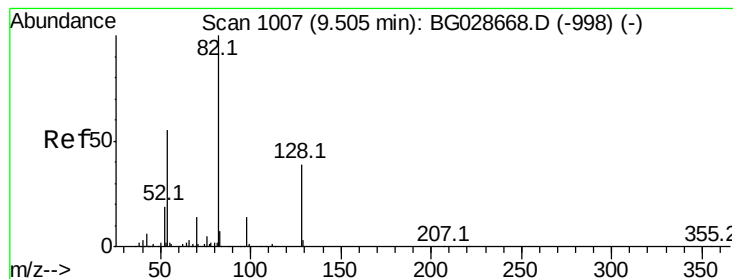

#23

Nitrobenzene-d5

Concen: 83.765 ng

RT: 9.50 min Scan# 1006

Delta R.T. -0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11

Instrument :

BNA_G

ClientSampleId :

PB102188BL





Tot Ion: 82 Resp: 213855

Ion Ratio Lower Upper

82 100

128 36.8 26.4 39.6

54 58.8 49.4 74.2

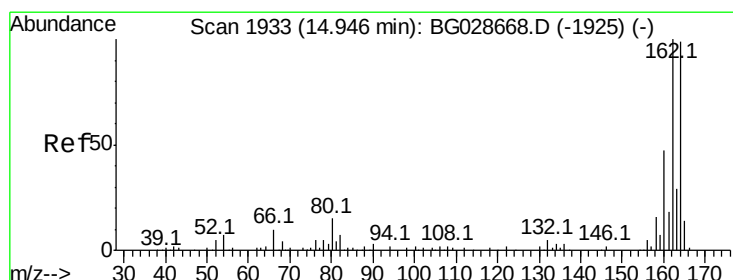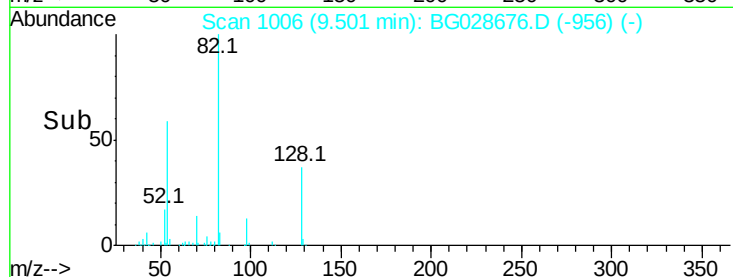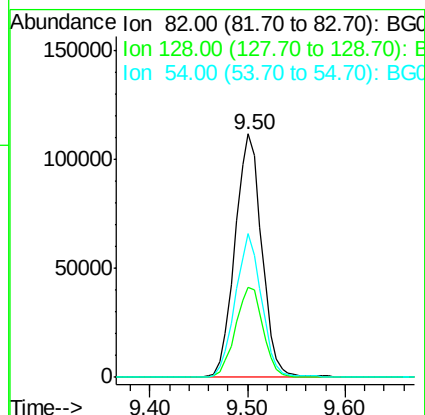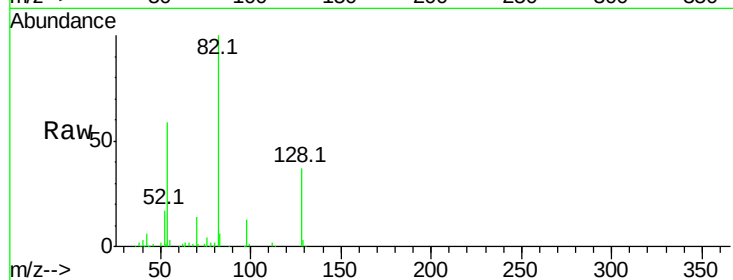

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.94 min Scan# 1932

Delta R.T. -0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11




Tgt Ion: 164 Resp: 88118


Ion Ratio Lower Upper

164 100

162 103.3 85.1 127.7

160 48.6 34.7 52.1

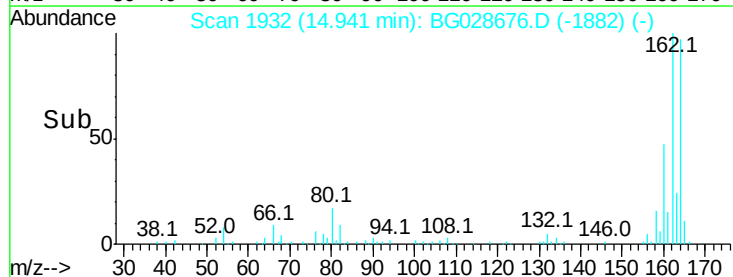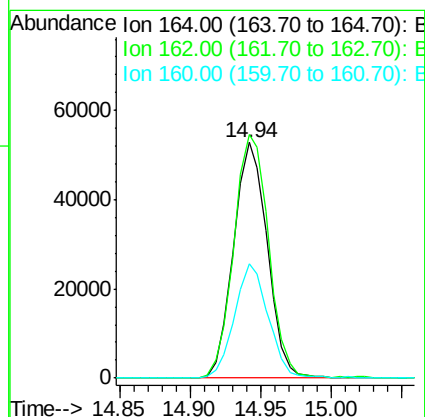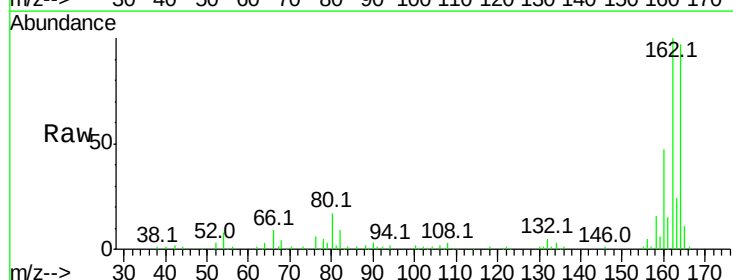


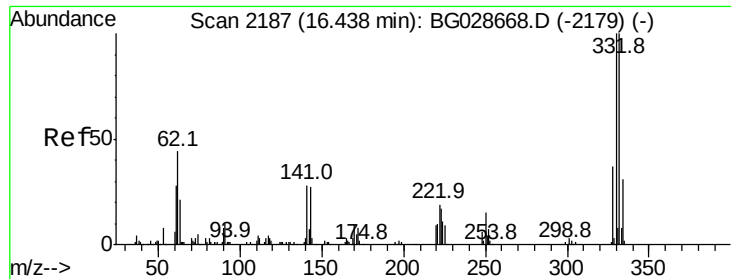




#41
 2,4,6-Tribromophenol
 Concen: 145.517 ng
 RT: 16.43 min Scan# 2186
 Delta R.T. -0.00 min
 Lab File: BG028676.D
 Acq: 12 Sep 2017 19:11

Instrument :
 BNA_G
 ClientSampleId :
 PB102188BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	77.3	115.9
141	30.5	32.1	48.1#

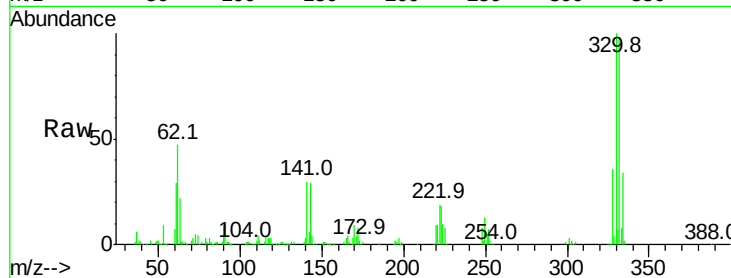


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

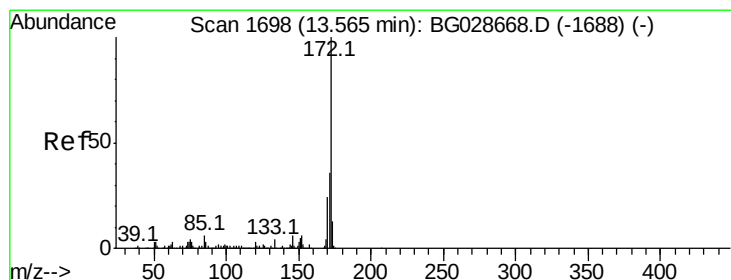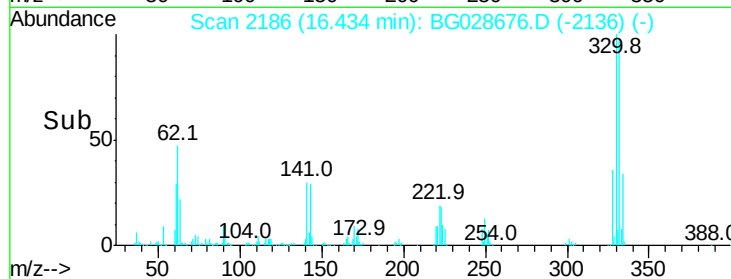
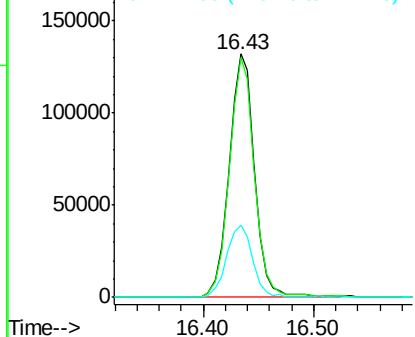



#44
 2-Fluorobiphenyl
 Concen: 84.573 ng
 RT: 13.56 min Scan# 1697
 Delta R.T. -0.00 min
 Lab File: BG028676.D
 Acq: 12 Sep 2017 19:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.1	32.2	48.2
170	23.7	21.8	32.6

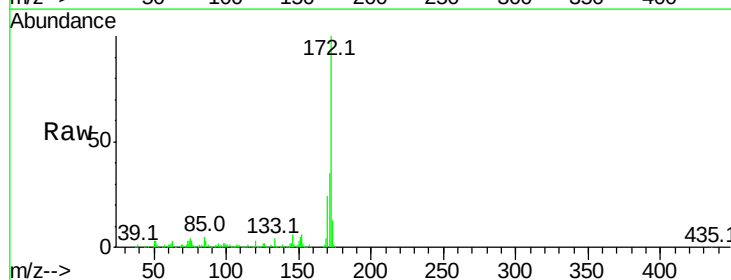

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

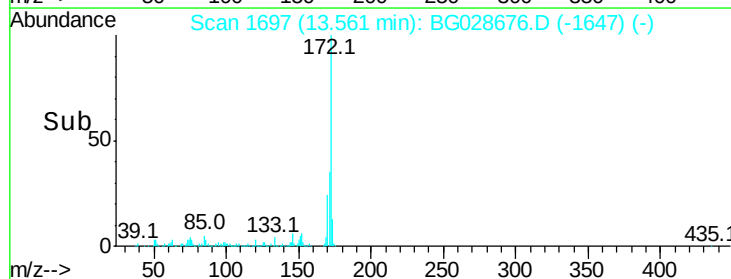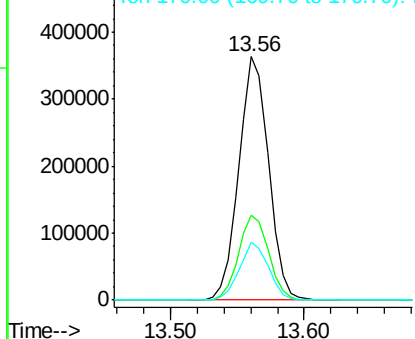

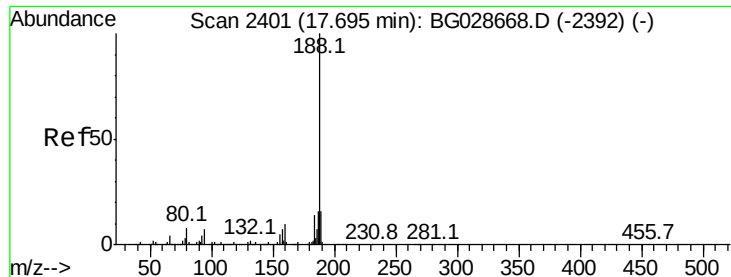

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.69 min Scan# 2400

Delta R.T. -0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11

Instrument :

BNA_G

ClientSampleId :

PB102188BL


Tot Ion:188 Resp: 265949

Ion Ratio Lower Upper

188 100

94 6.6 5.8 8.8

80 7.9 7.5 11.3

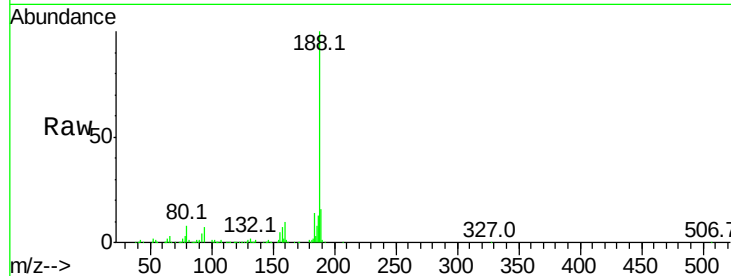

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

200000

150000

100000

50000

0



17.69

17.60

17.70

17.80

Time-->

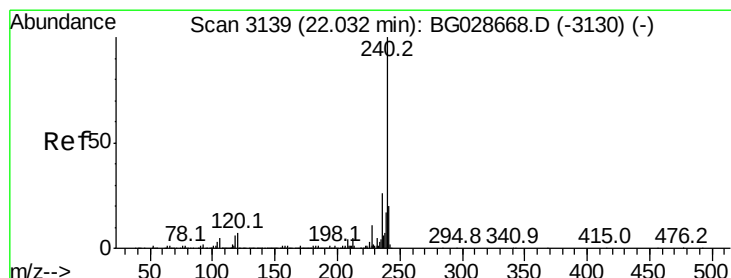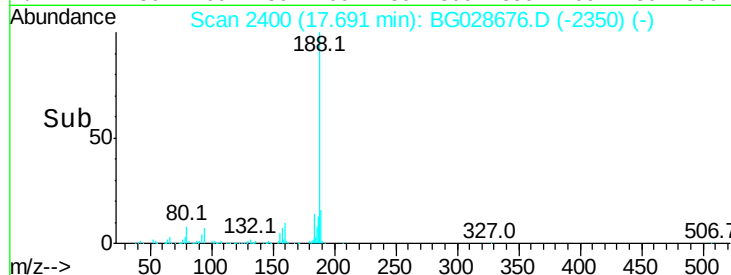

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.03 min Scan# 3138

Delta R.T. -0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11


Tgt Ion:240 Resp: 304193

Ion Ratio Lower Upper

240 100

120 6.2 5.7 8.5

236 26.3 22.2 33.4

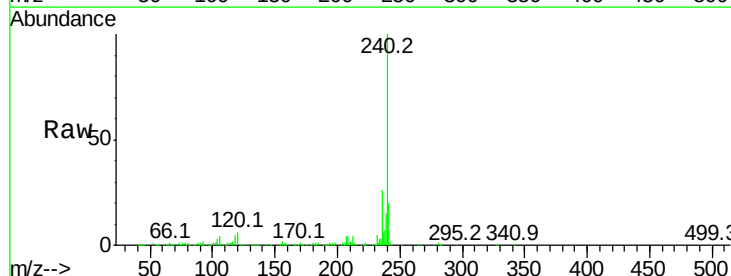

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

200000

150000

100000

50000

0


22.03


21.90

22.00

22.10

Time-->

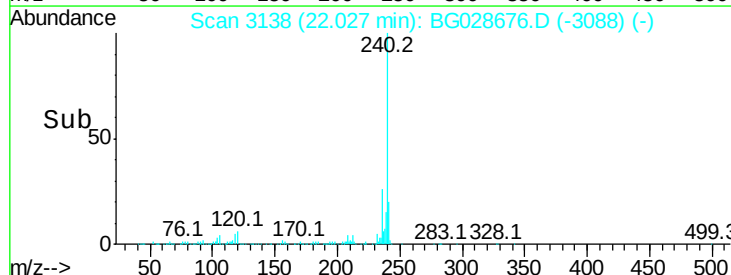

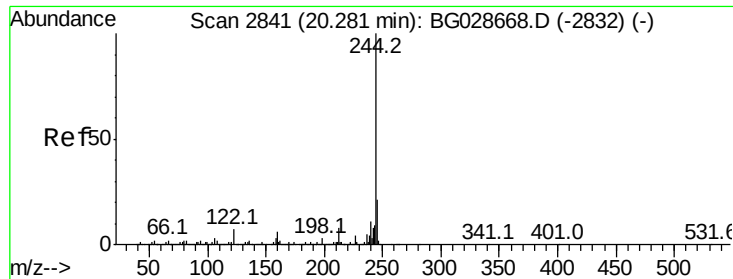

#78

Terphenyl-d14

Concen: 79.132 ng

RT: 20.28 min Scan# 2840

Delta R.T. -0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11

Instrument :

BNA_G

ClientSampleId :

PB102188BL





Tot Ion:244 Resp: 1128759

Ion Ratio Lower Upper

244 100

212 7.6 10.0 15.0#

122 7.6 8.6 12.8#

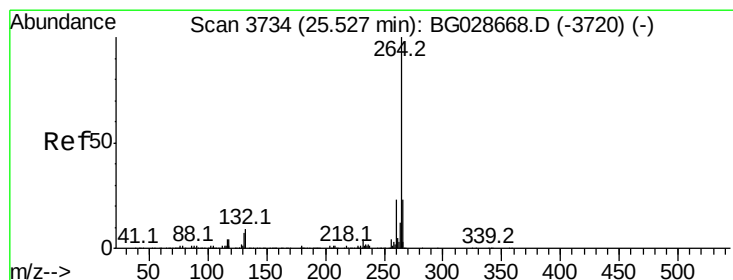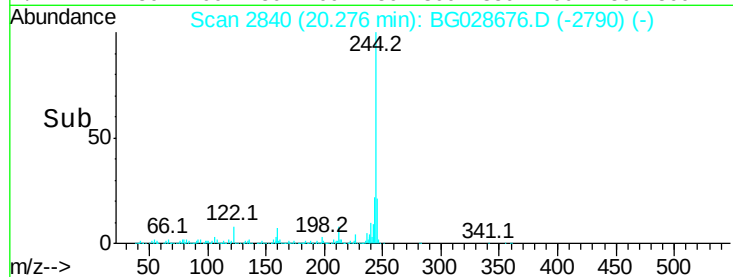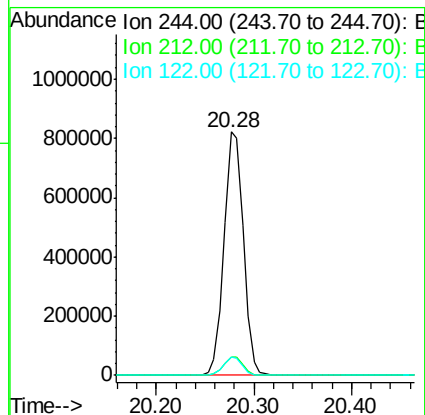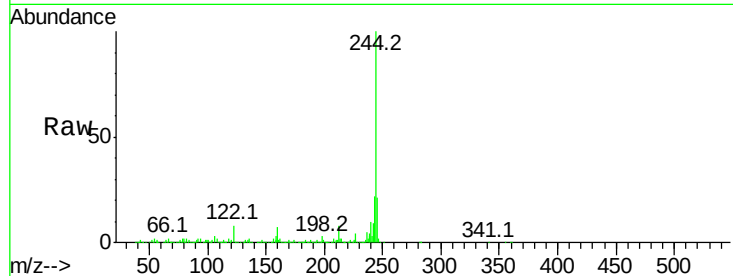

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.53 min Scan# 3734

Delta R.T. 0.00 min

Lab File: BG028676.D

Acq: 12 Sep 2017 19:11

Tgt Ion:264 Resp: 313811

Ion Ratio Lower Upper

264 100

260 21.6 21.8 32.8#

265 20.5 18.2 27.4

