


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG091217\
 Data File : BG028664.D
 Acq On : 12 Sep 2017 11:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

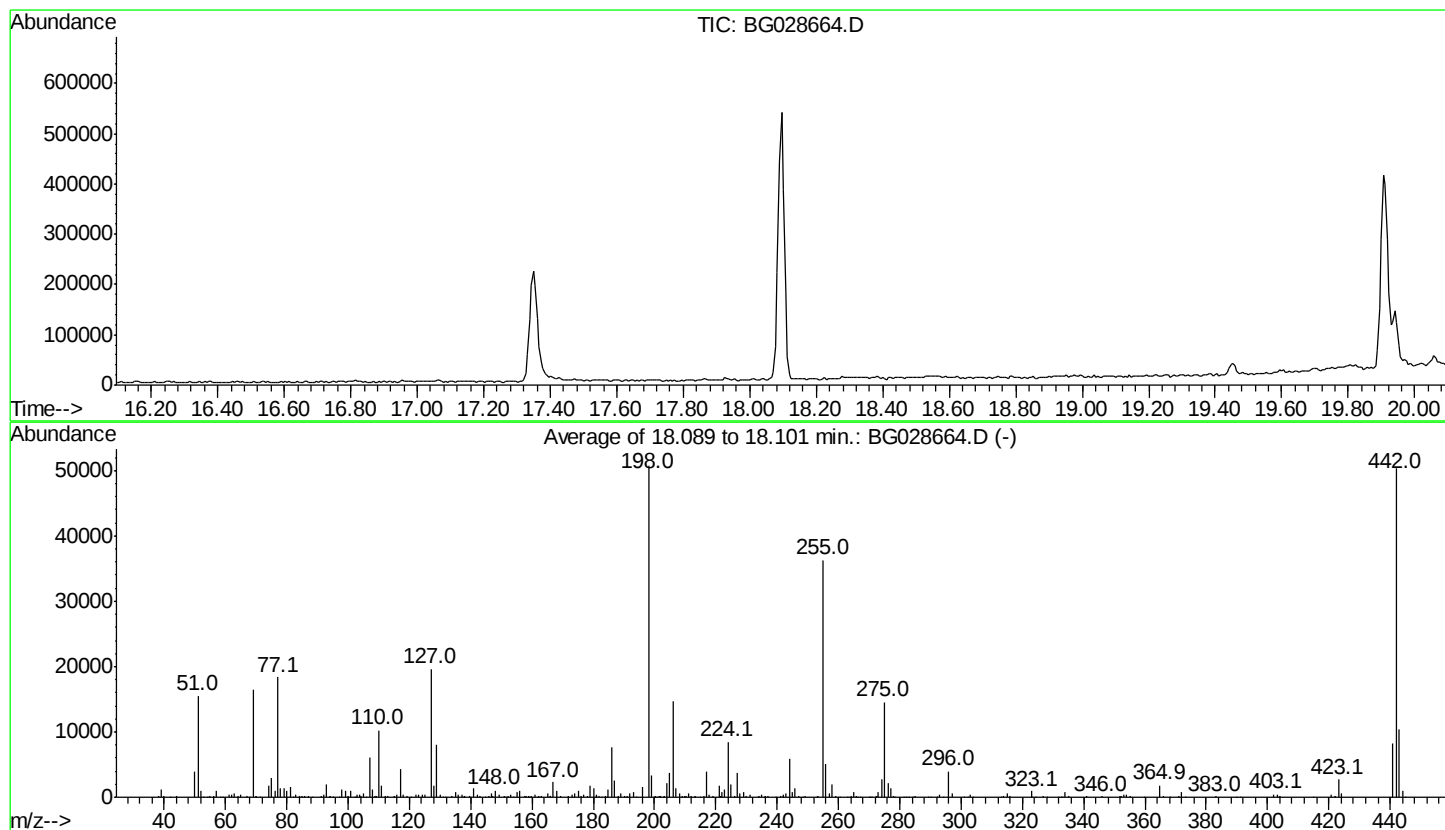

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	15547	PASS
68	69	0.00	2	0.2	37	PASS
69	198	0.00	100	32.6	16560	PASS
70	69	0.00	2	1.0	159	PASS
127	198	10	80	38.7	19644	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50754	PASS
199	198	5	9	6.7	3424	PASS
275	198	10	60	28.7	14544	PASS
365	198	1	100	3.6	1807	PASS
441	442	0.01	24	16.3	8218	PASS
442	198	50	100	99.4	50426	PASS
443	442	15	24	20.4	10297	PASS