


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG091217\
 Data File : BG028673.D
 Acq On : 12 Sep 2017 17:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

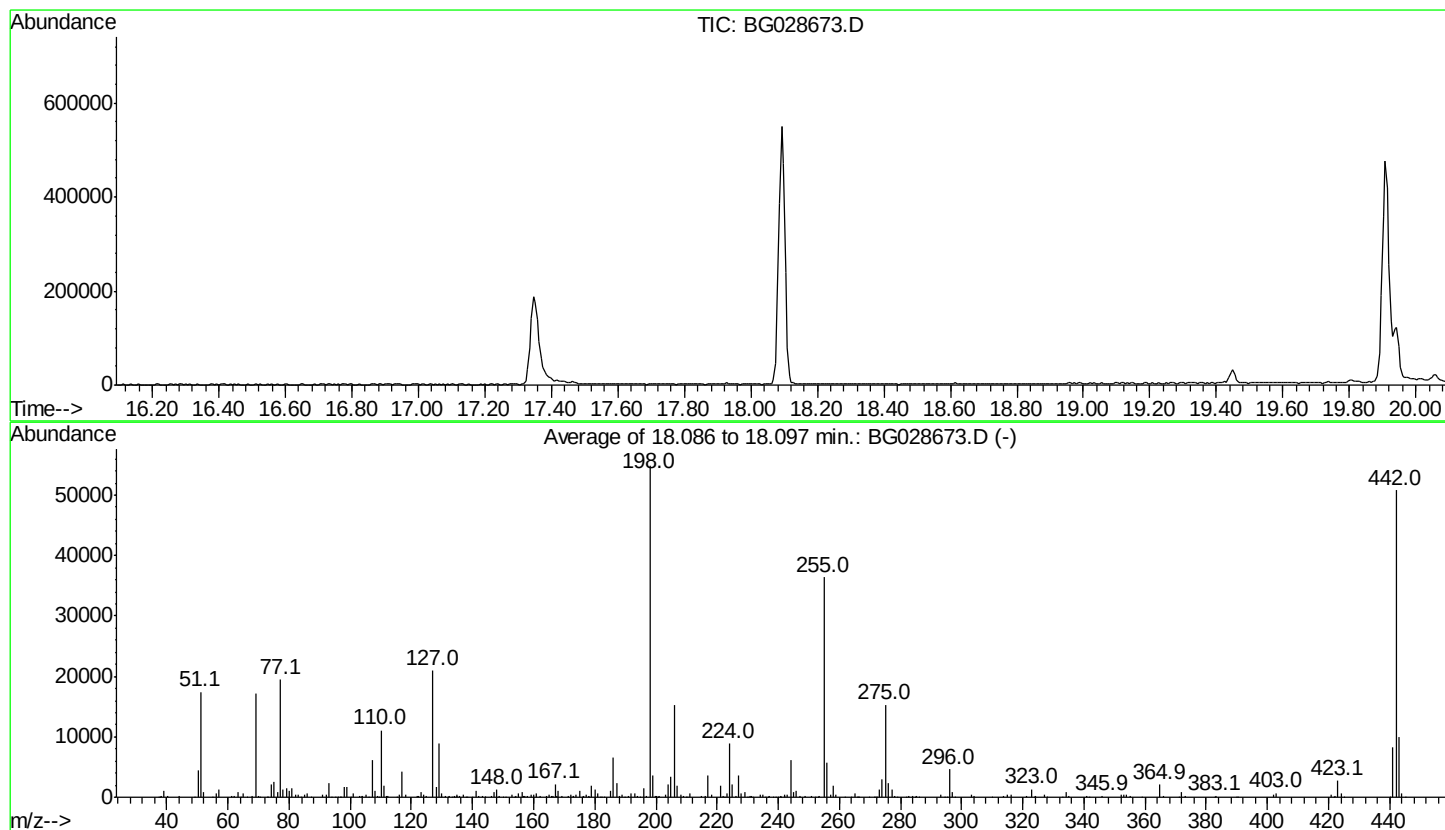

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	17442	PASS
68	69	0.00	2	1.4	245	PASS
69	198	0.00	100	31.3	17191	PASS
70	69	0.00	2	0.8	142	PASS
127	198	10	80	38.2	20954	PASS
197	198	0.00	2	0.3	175	PASS
198	198	100	100	100.0	54885	PASS
199	198	5	9	6.6	3602	PASS
275	198	10	60	27.9	15334	PASS
365	198	1	100	3.8	2069	PASS
441	442	0.01	24	16.4	8322	PASS
442	198	50	100	92.6	50808	PASS
443	442	15	24	19.8	10041	PASS