
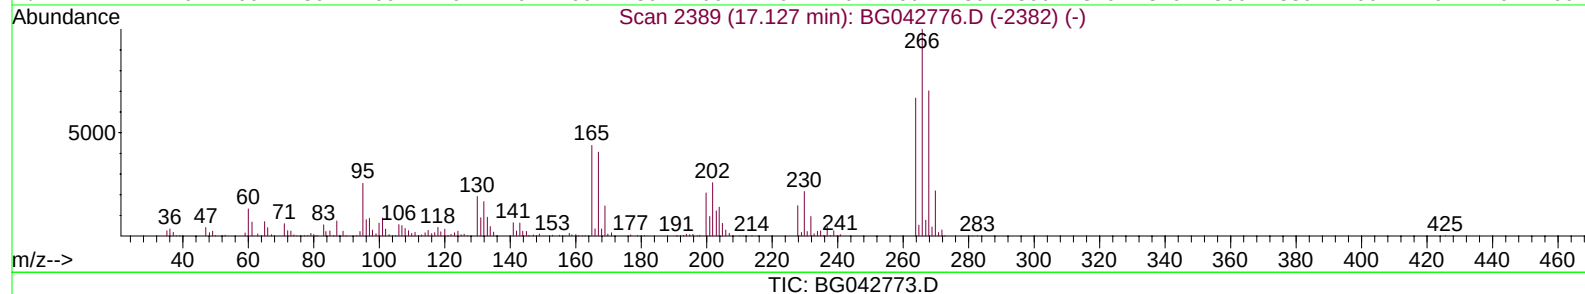
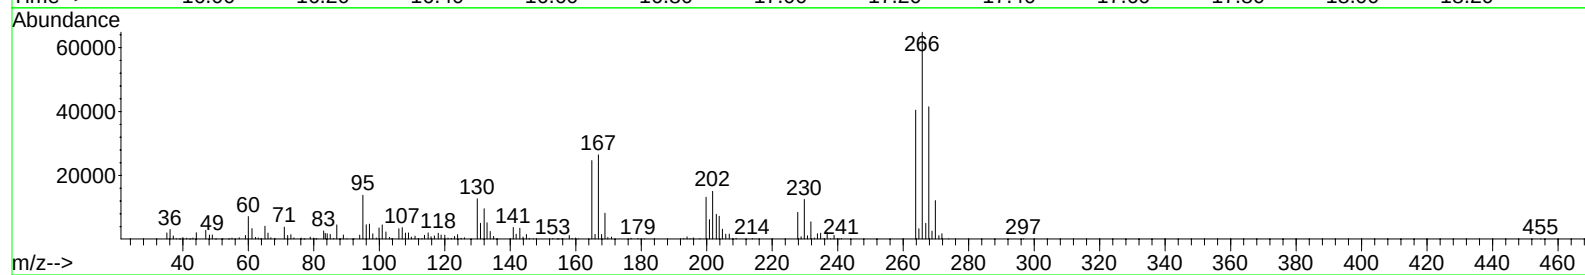


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091219\
Data File : BG042773.D
Acq On : 12 Sep 2019 8:37
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 18:35:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG091219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 14:06:09 2019
Response via : Initial Calibration

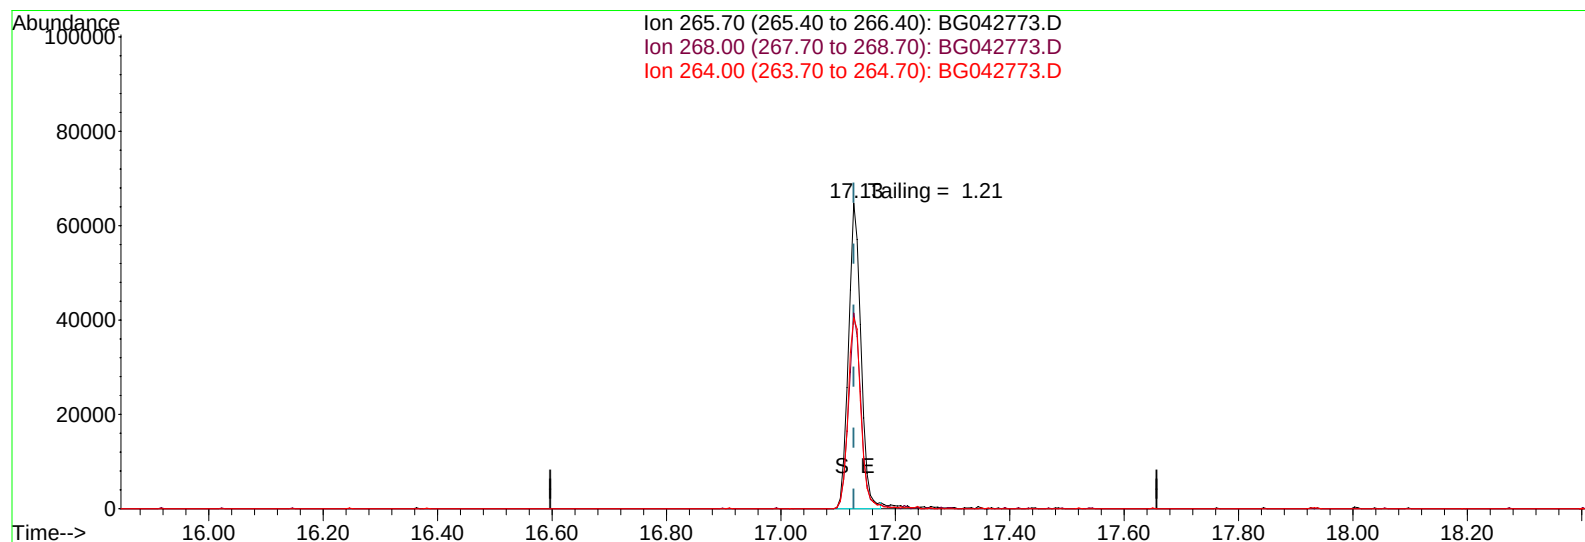

TIC: BG042773.D

(70) Pentachlorophenol (C)




17.127min (+0.000) 211285.15ng

response 100505

Ion	Exp%	Act%
265.70	100	100
268.00	70.30	64.00
264.00	66.80	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091219\
Data File : BG042773.D
Acq On : 12 Sep 2019 8:37
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 18:35:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG091219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 14:06:09 2019
Response via : Initial Calibration

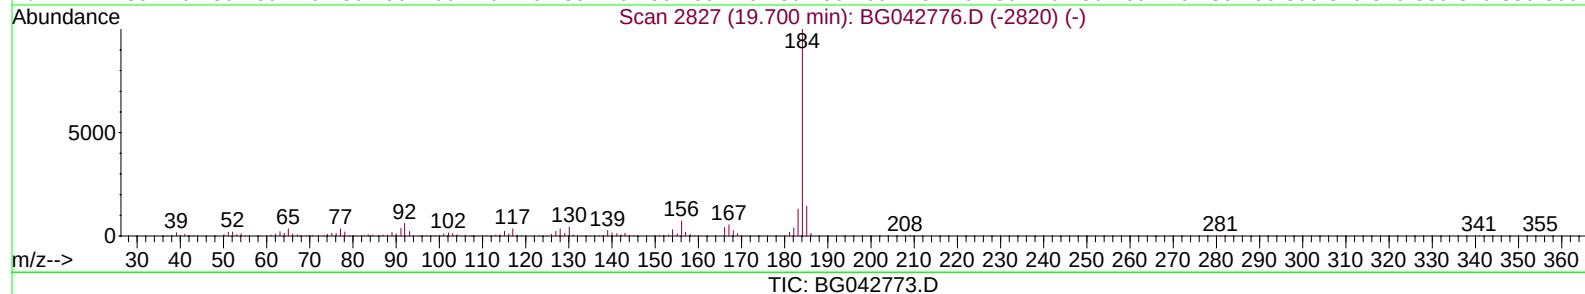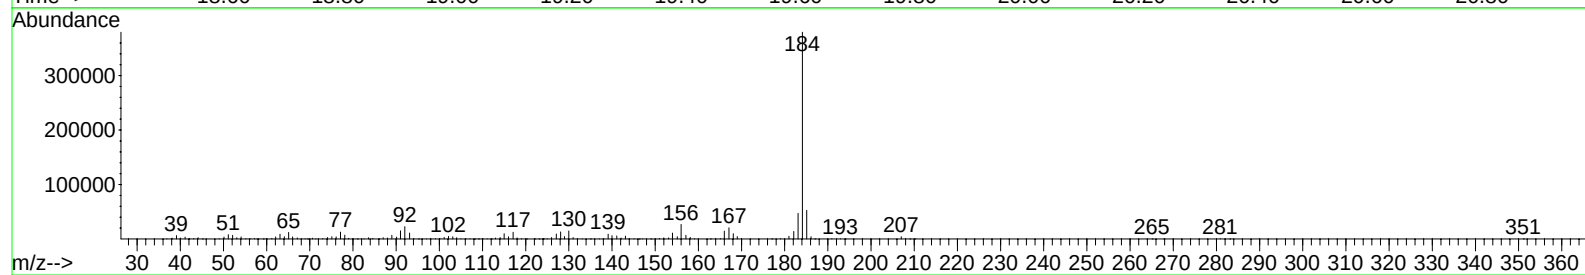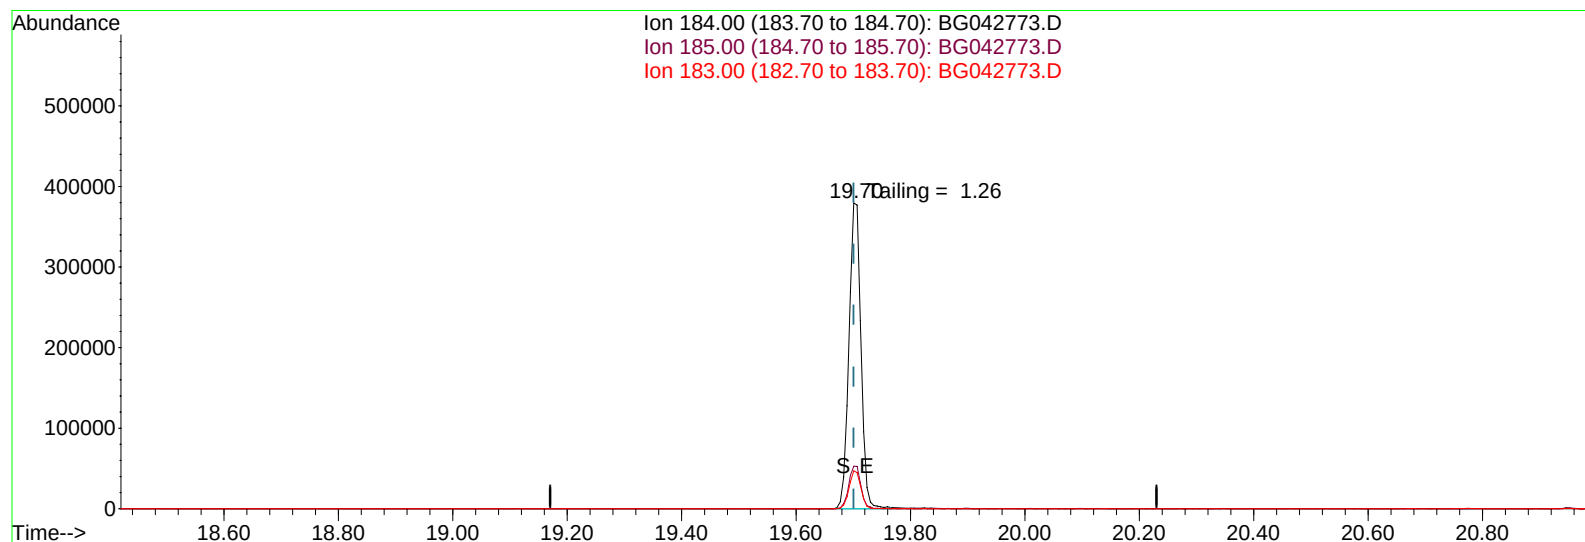

(77) Benzidine

19.701min (+0.000) 377670.33ng

response 559238

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	13.92
183.00	13.00	12.39
0.00	0.00	0.00