


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG091219\  
 Data File : BG042773.D  
 Acq On : 12 Sep 2019 8:37  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG091219.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Sep 12 14:06:09 2019

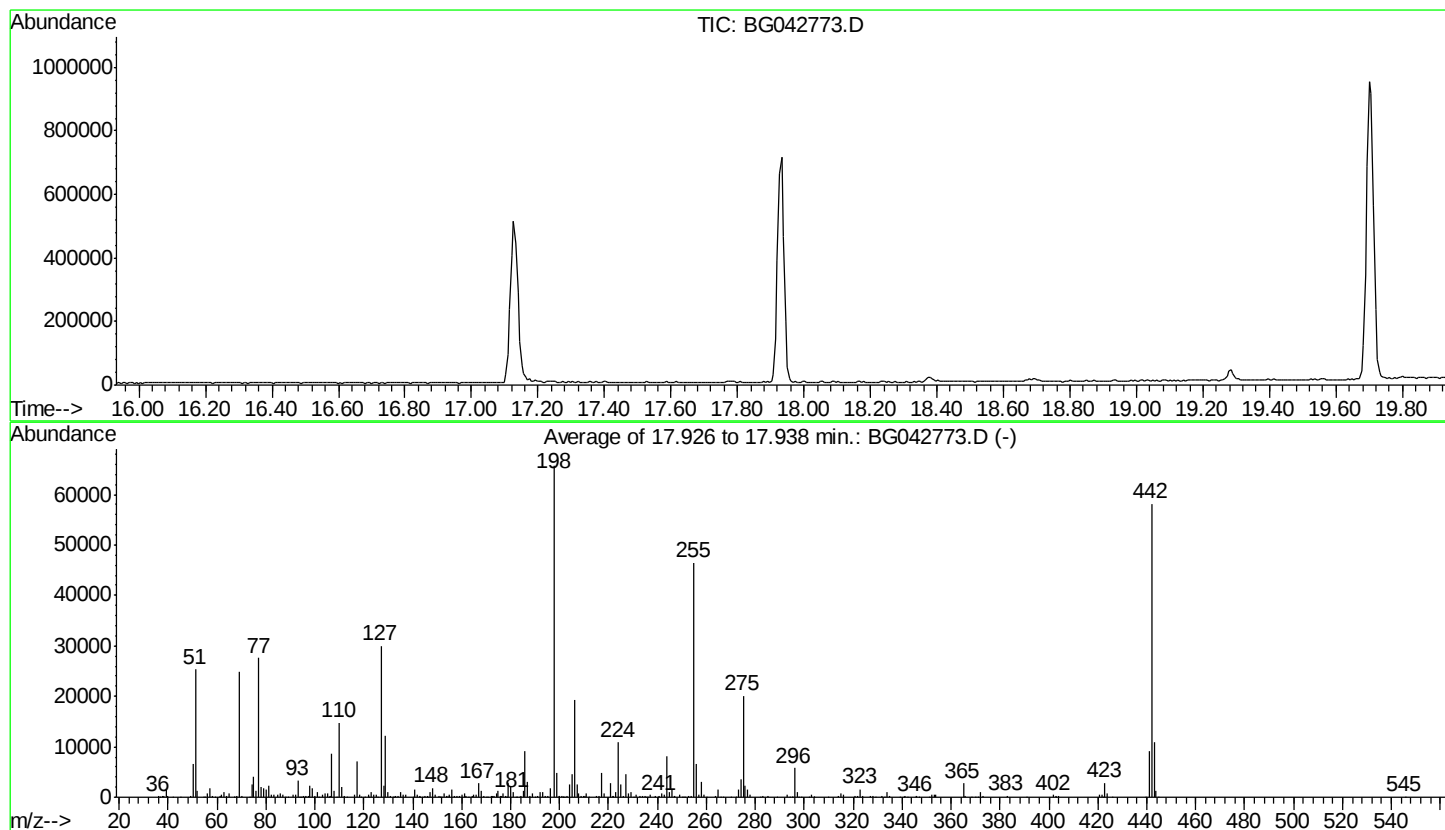

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 38.5      | 25328   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.9       | 231     | PASS             |
| 69          | 198          | 0.00         | 100          | 37.9      | 24898   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.8       | 211     | PASS             |
| 127         | 198          | 10           | 80           | 45.7      | 30053   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 65728   | PASS             |
| 199         | 198          | 5            | 9            | 7.2       | 4718    | PASS             |
| 275         | 198          | 10           | 60           | 30.6      | 20091   | PASS             |
| 365         | 198          | 1            | 100          | 4.2       | 2757    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.9      | 9133    | PASS             |
| 442         | 198          | 50           | 100          | 88.5      | 58152   | PASS             |
| 443         | 442          | 15           | 24           | 19.0      | 11035   | PASS             |