


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091219\
 Data File : BG042782.D
 Acq On : 12 Sep 2019 15:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:06:09 2019

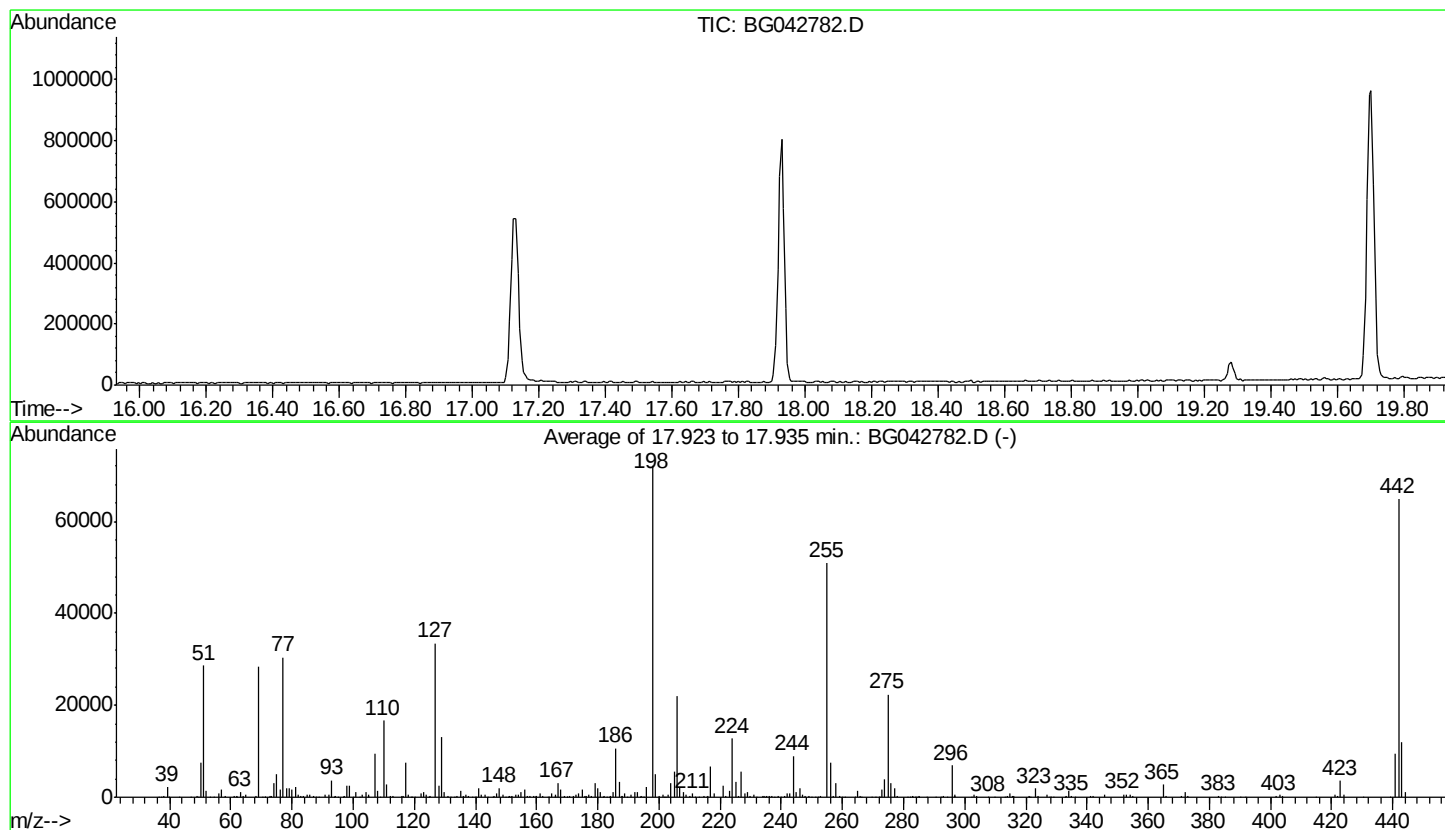

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	28618	PASS
68	69	0.00	2	0.5	150	PASS
69	198	0.00	100	39.6	28525	PASS
70	69	0.00	2	0.4	122	PASS
127	198	10	80	46.5	33544	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72122	PASS
199	198	5	9	7.0	5030	PASS
275	198	10	60	30.9	22298	PASS
365	198	1	100	3.9	2783	PASS
441	198	0.01	100	13.2	9500	PASS
442	198	50	100	90.1	64984	PASS
443	442	15	24	18.5	12039	PASS