


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091219\
Data File : BG042800.D
Acq On : 13 Sep 2019 3:52
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG091219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 12 14:06:09 2019

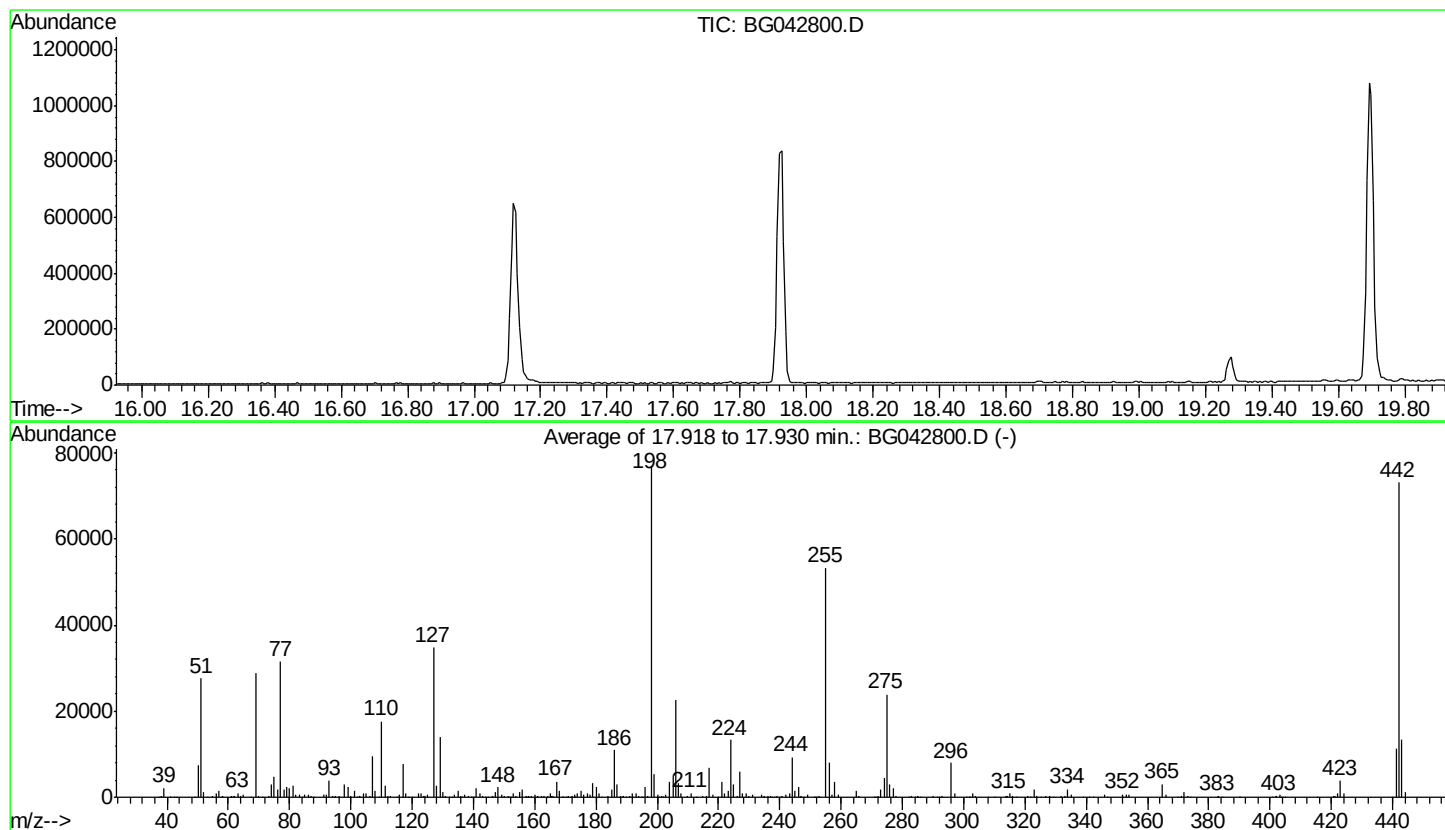

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	27642	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.5	28925	PASS
70	69	0.00	2	1.2	352	PASS
127	198	10	80	45.2	34781	PASS
197	198	0.00	2	0.4	320	PASS
198	198	100	100	100.0	77032	PASS
199	198	5	9	6.8	5262	PASS
275	198	10	60	31.0	23874	PASS
365	198	1	100	3.9	2994	PASS
441	198	0.01	100	14.8	11367	PASS
442	198	50	100	94.9	73088	PASS
443	442	15	24	18.4	13477	PASS