
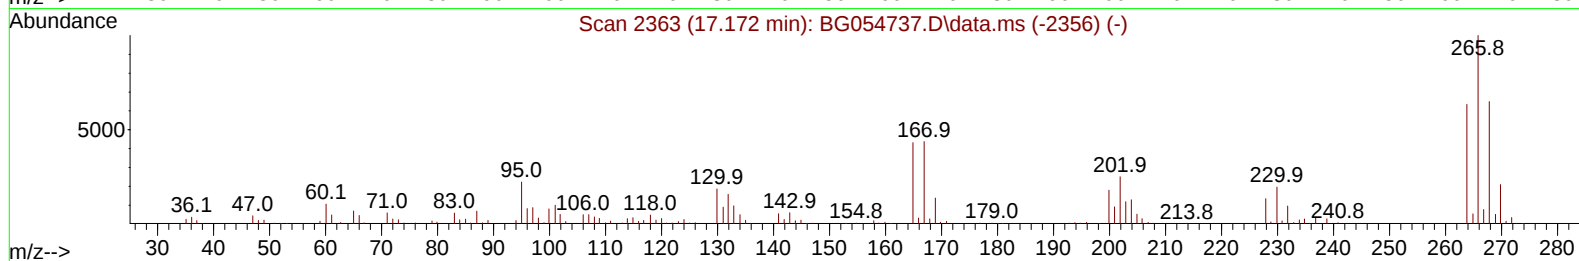
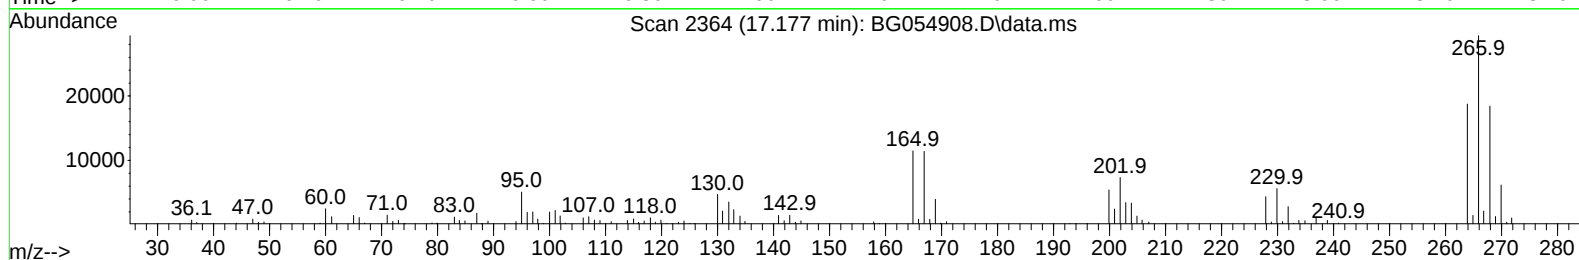


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091222\
Data File : BG054908.D
Acq On : 12 Sep 2022 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 13:58:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

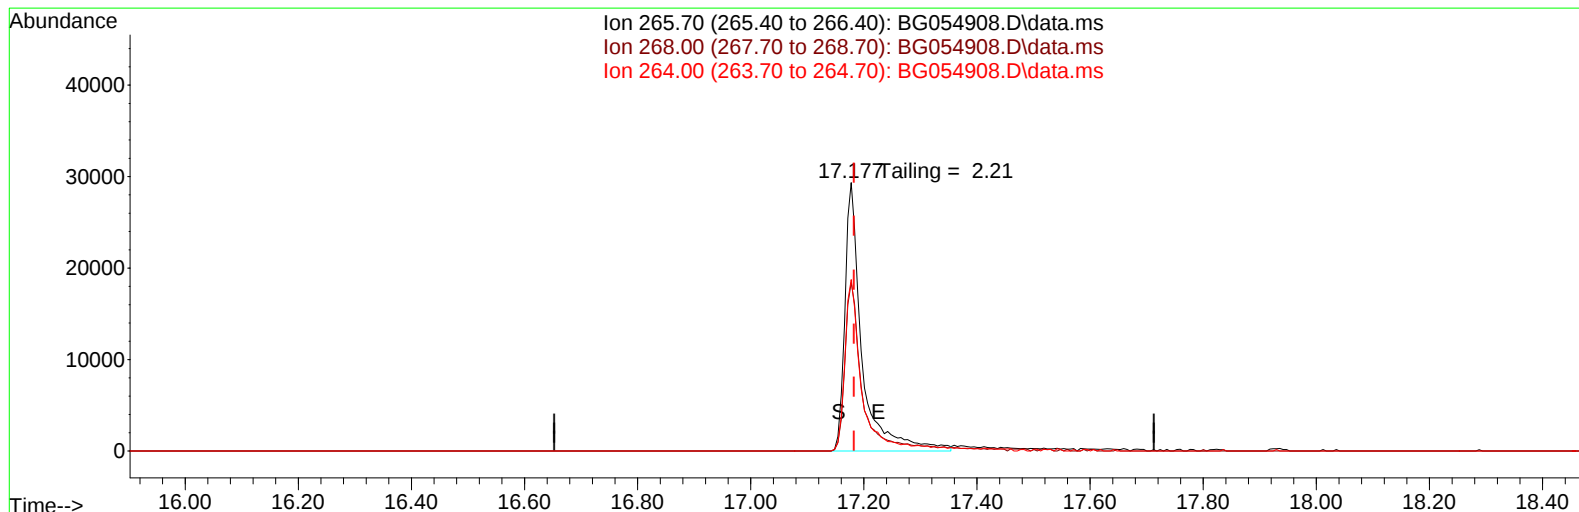

TIC: BG054908.D\data.ms

(70) Pentachlorophenol (C)




17.177min (-0.005) 28565.51 ng

response 61300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.76
264.00	61.70	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091222\
Data File : BG054908.D
Acq On : 12 Sep 2022 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 13:58:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

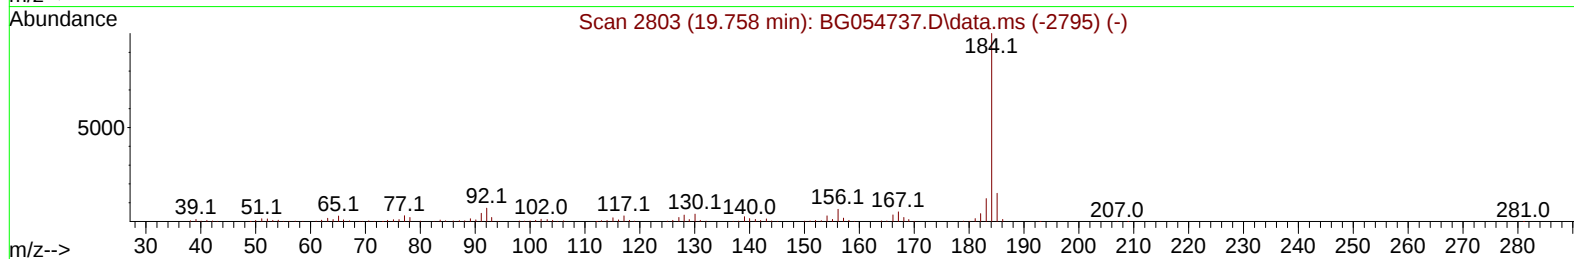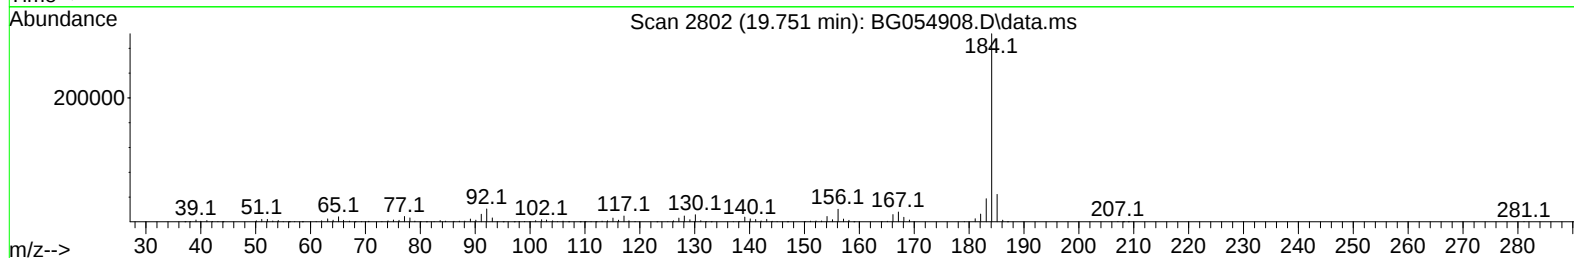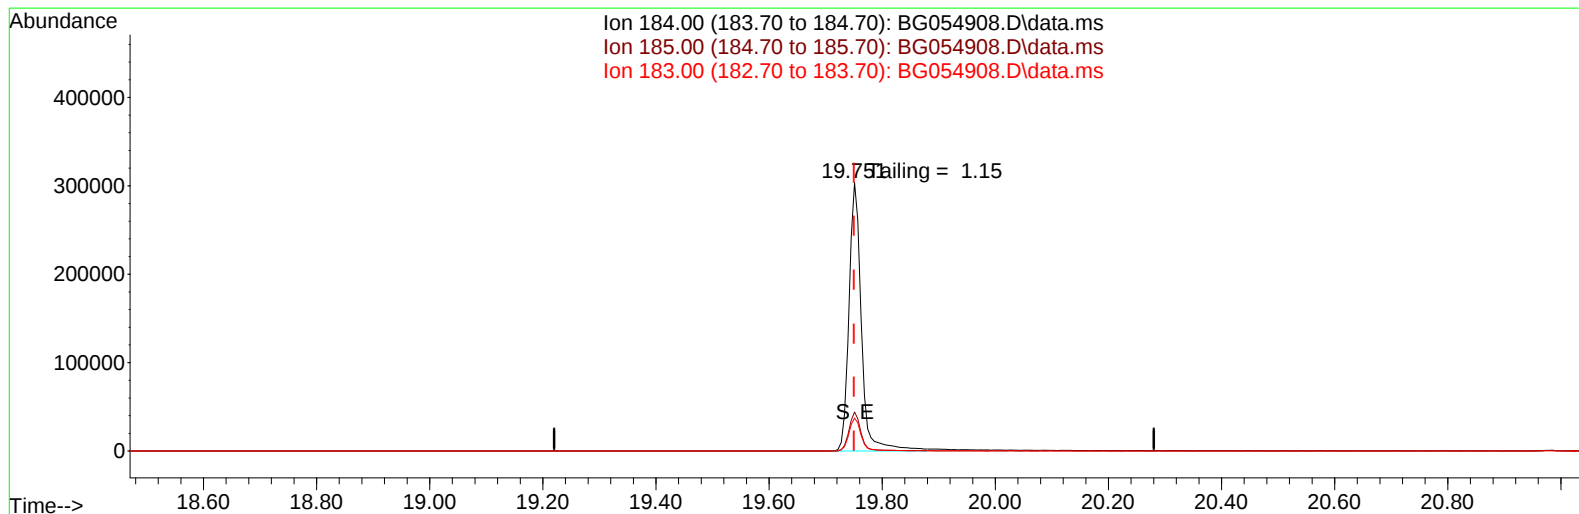

TIC: BG054908.D\data.ms

(77) Benzidine

19.751min (+ 0.001) 0.00 ng

response 472391

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.56
183.00	12.30	12.32
0.00	0.00	0.00