

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091222\
 Data File : BG054921.D
 Acq On : 13 Sep 2022 1:14
 Operator : CG/JU
 Sample : N4562-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CHRT-26524

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.502	32	36	43	rVB	18269	29303	1.51%	0.279%
2	4.695	234	239	246	rBV	13461	23014	1.19%	0.219%
3	5.206	318	326	334	rBV	51507	85023	4.39%	0.810%
4	5.694	401	409	421	rBV	512405	901116	46.57%	8.585%
5	7.310	674	684	694	rBV	526069	944458	48.81%	8.998%
6	8.144	820	826	840	rVB	143782	257472	13.31%	2.453%
7	9.319	1018	1026	1037	rBV	318043	611953	31.62%	5.830%
8	10.723	1259	1265	1274	rBV3	8986	20680	1.07%	0.197%
9	10.911	1290	1297	1301	rBV2	12524	21737	1.12%	0.207%
10	10.970	1301	1307	1315	rBV	194972	365384	18.88%	3.481%
11	12.351	1536	1542	1548	rBV2	14709	23329	1.21%	0.222%
12	13.291	1697	1702	1710	rVB4	10162	20547	1.06%	0.196%
13	13.403	1714	1721	1730	rVV	978562	1533518	79.25%	14.610%
14	13.573	1743	1750	1756	rBV3	25988	52247	2.70%	0.498%
15	14.196	1851	1856	1860	rBV2	35421	55946	2.89%	0.533%
16	14.513	1905	1910	1914	rBV5	31159	55424	2.86%	0.528%
17	14.601	1921	1925	1929	rVB2	49549	70667	3.65%	0.673%
18	14.783	1950	1956	1962	rVB	301929	508579	26.28%	4.845%
19	14.848	1963	1967	1975	rBV5	23778	51644	2.67%	0.492%
20	15.494	2073	2077	2082	rVB5	25075	43179	2.23%	0.411%
21	15.559	2084	2088	2092	rVV	70235	98545	5.09%	0.939%
22	16.270	2204	2209	2217	rBV	628813	1005934	51.98%	9.584%
23	16.710	2281	2284	2288	rBV2	50395	70203	3.63%	0.669%
24	17.533	2419	2424	2428	rBV	340083	514076	26.57%	4.898%
25	19.584	2769	2773	2776	rBV	227680	295285	15.26%	2.813%
26	19.942	2831	2834	2843	rVB	306031	444728	22.98%	4.237%
27	20.130	2861	2866	2872	rVB	1460435	1935057	100.00%	18.435%
28	21.681	3126	3130	3137	rVB	314076	457394	23.64%	4.358%




Sum of corrected areas: 10496442

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091222\
Data File : BG054921.D
Acq On : 13 Sep 2022 1:14
Operator : CG/JU
Sample : N4562-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHRT-26524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

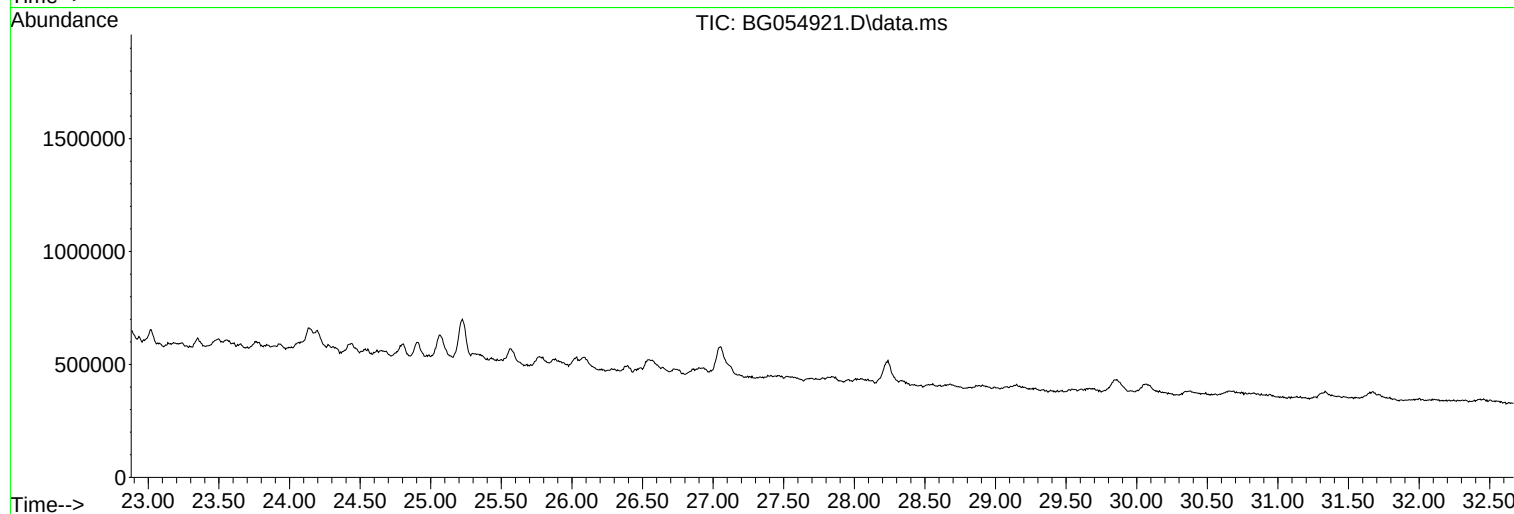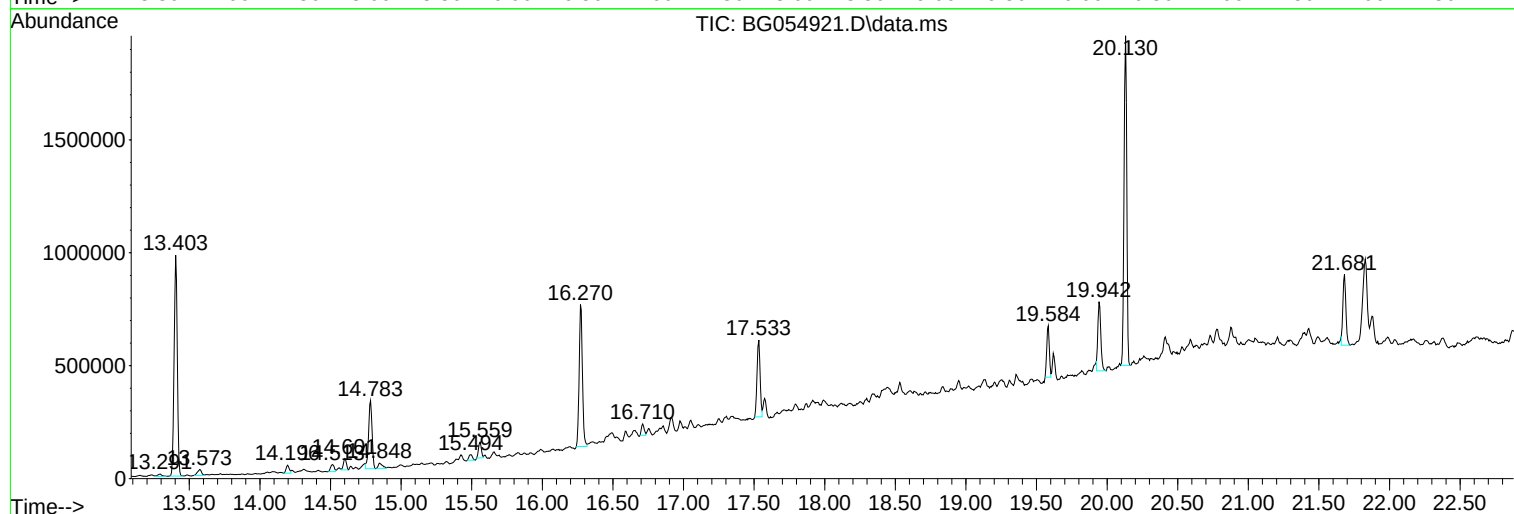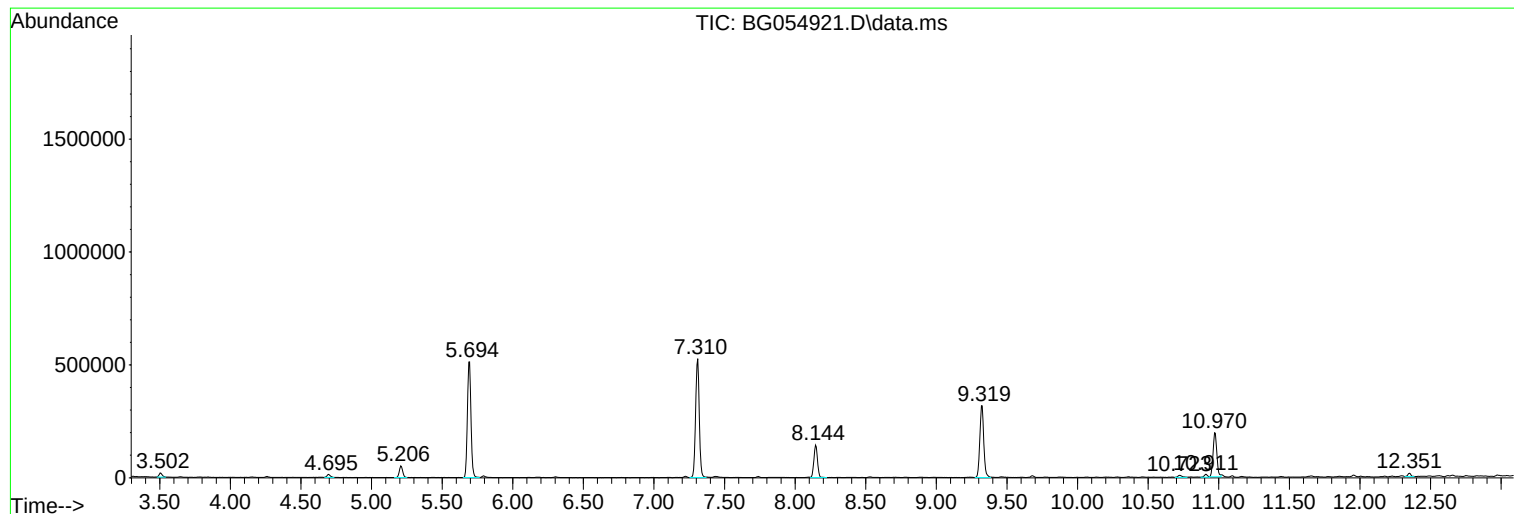

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091222\
Data File : BG054921.D
Acq On : 13 Sep 2022 1:14
Operator : CG/JU
Sample : N4562-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHRT-26524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091222\
Data File : BG054921.D
Acq On : 13 Sep 2022 1:14
Operator : CG/JU
Sample : N4562-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHRT-26524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------