




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
Data File : BG062764.D
Acq On : 12 Sep 2024 15:46
Operator : JU/RC
Sample : P3922-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AS9

Manual IntegrationsAPPROVED

Quant Time: Sep 12 16:27:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/13/2024
Supervised By :mohammad ahmed 09/14/2024

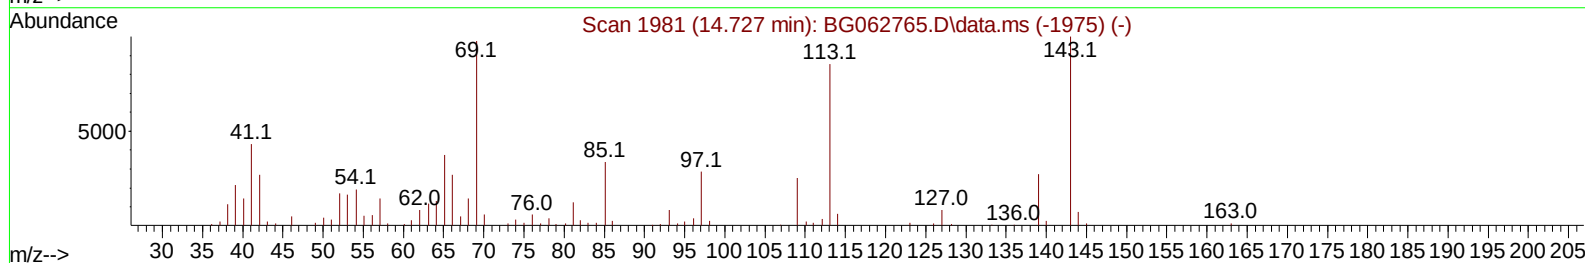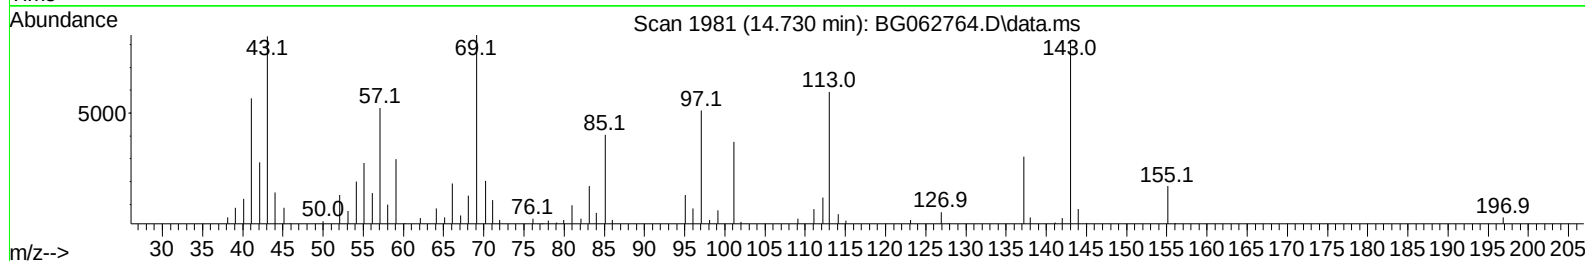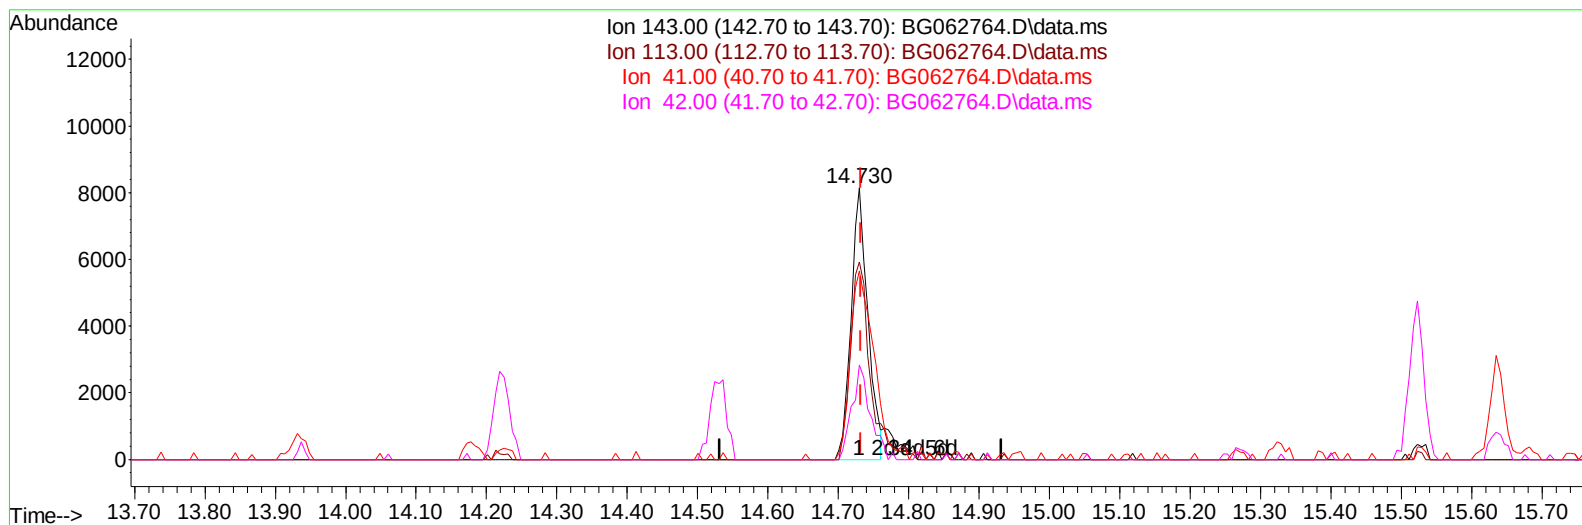

TIC: BG062764.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.730min (-0.002) 7.20 ng/ul

response 13398

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.40	72.66
41.00	45.80	69.38#
42.00	31.60	34.82




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
Data File : BG062764.D
Acq On : 12 Sep 2024 15:46
Operator : JU/RC
Sample : P3922-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AS9

Manual IntegrationsAPPROVED

Quant Time: Sep 12 16:27:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/13/2024
Supervised By :mohammad ahmed 09/14/2024

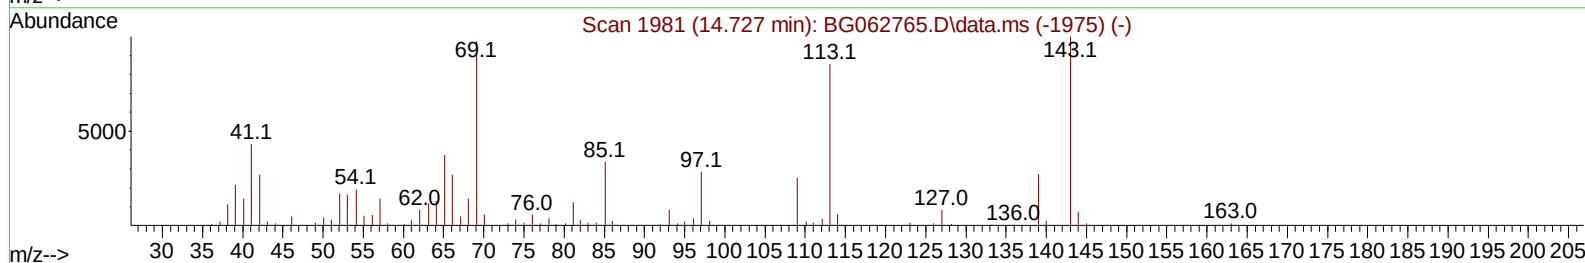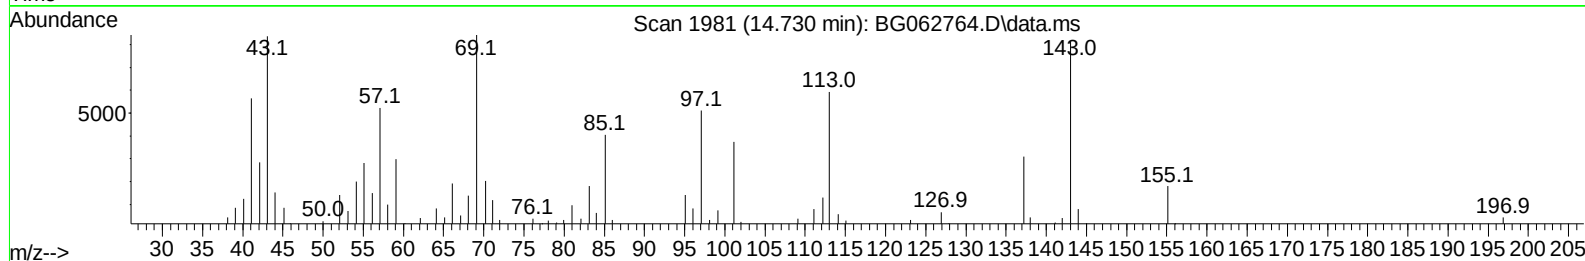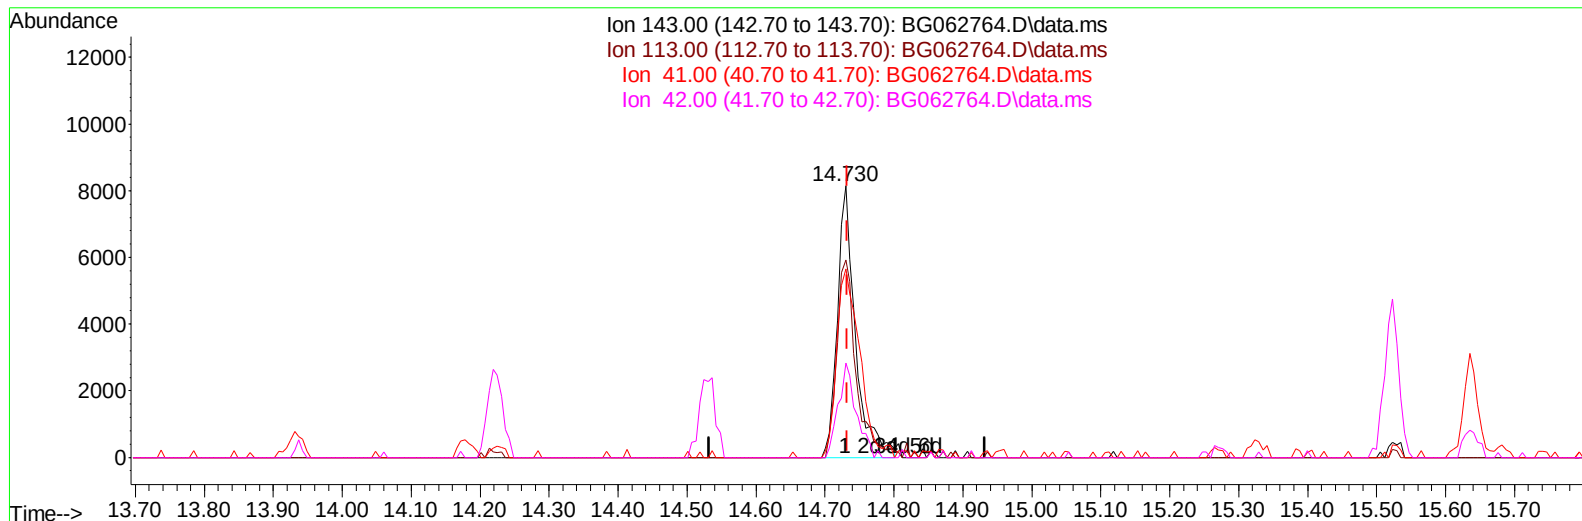

TIC: BG062764.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.730min (-0.002) 7.95 ng/ul m

response 14792

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.40	72.66
41.00	45.80	69.38#
42.00	31.60	34.82

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
 Data File : BG062764.D
 Acq On : 12 Sep 2024 15:46
 Operator : JU/RC
 Sample : P3922-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AS9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/13/2024
 Supervised By :mohammad ahmed 09/14/2024

Quant Time: Sep 13 00:03:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.903	152	38488	20.000	ng/ul	0.00
20) Naphthalene-d8	10.694	136	175084	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.530	164	142159	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.274	188	376789	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	416786	20.000	ng/ul	0.00
88) Perylene-d12	24.583	264	453686	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.361	96	4730	5.555	ng/uL	0.00
4) Pyridine-d5	3.772	84	14735	5.437	ng/ul	0.00
7) Phenol-d5	7.069	99	31848	9.437	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.227	67	53684	26.531	ng/ul	0.00
11) 2-Chlorophenol-d4	7.433	132	64776	26.350	ng/ul	0.00
15) 4-Methylphenol-d8	8.608	113	61052	21.708	ng/ul	0.00
21) Nitrobenzene-d5	9.054	128	36578	29.231	ng/ul	0.00
24) 2-Nitrophenol-d4	9.777	143	42037	30.717	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.318	165	84279	28.278	ng/ul	0.00
31) 4-Chloroaniline-d4	10.829	131	81870	19.984	ng/ul	0.00
46) Dimethylphthalate-d6	13.937	166	323982	29.595	ng/ul	0.00
49) Acenaphthylene-d8	14.225	160	344475	28.333	ng/ul	0.00
54) 4-Nitrophenol-d4	14.730	143	14792m	7.954	ng/ul	0.00
60) Fluorene-d10	15.523	176	305889	31.008	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.635	200	59553	27.477	ng/ul	0.00
73) Anthracene-d10	17.374	188	630607	35.463	ng/ul	0.00
81) Pyrene-d10	19.666	212	820770	34.995	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.372	264	873797	36.475	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
Data File : BG062764.D
Acq On : 12 Sep 2024 15:46
Operator : JU/RC
Sample : P3922-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AS9

Manual IntegrationsAPPROVED

Quant Time: Sep 13 00:03:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/13/2024
Supervised By :mohammad ahmed 09/14/2024

