

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
 Data File : BG062771.D
 Acq On : 12 Sep 2024 21:00
 Operator : JU/RC
 Sample : P3877-15DL 30X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCVZ4DL

Quant Time: Sep 12 23:31:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.906	152	46818	20.000	ng/u1	0.00
20) Naphthalene-d8	10.697	136	208927	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.528	164	196229	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.277	188	506829	20.000	ng/u1	0.00
79) Chrysene-d12	21.519	240	542974	20.000	ng/u1	0.00
88) Perylene-d12	24.580	264	605974	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.077	99	2767	0.674	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.230	67	1733	0.704	ng/u1	0.00
11) 2-Chlorophenol-d4	7.436	132	2103	0.703	ng/u1	0.00
15) 4-Methylphenol-d8	8.611	113	2362	0.690	ng/u1	0.00
21) Nitrobenzene-d5	9.052	128	854	0.572	ng/u1	0.00
24) 2-Nitrophenol-d4	9.780	143	1082	0.663	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.327	165	2734	0.769	ng/u1	0.00
31) 4-Chloroaniline-d4	10.832	131	3241	0.663	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	11503	0.761	ng/u1	0.00
49) Acenaphthylene-d8	14.222	160	12859	0.766	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.520	176	11398	0.837	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.371	188	20440	0.855	ng/u1	0.00
81) Pyrene-d10	19.663	212	25344	0.829	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.369	264	25997	0.812	ng/u1	-0.01
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.156	232	5684	1.278	ng/u1#	92
71) Pentachlorophenol	16.931	266	63014	15.821	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
Data File : BG062771.D
Acq On : 12 Sep 2024 21:00
Operator : JU/RC
Sample : P3877-15DL 30X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ4DL

Quant Time: Sep 12 23:31:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration




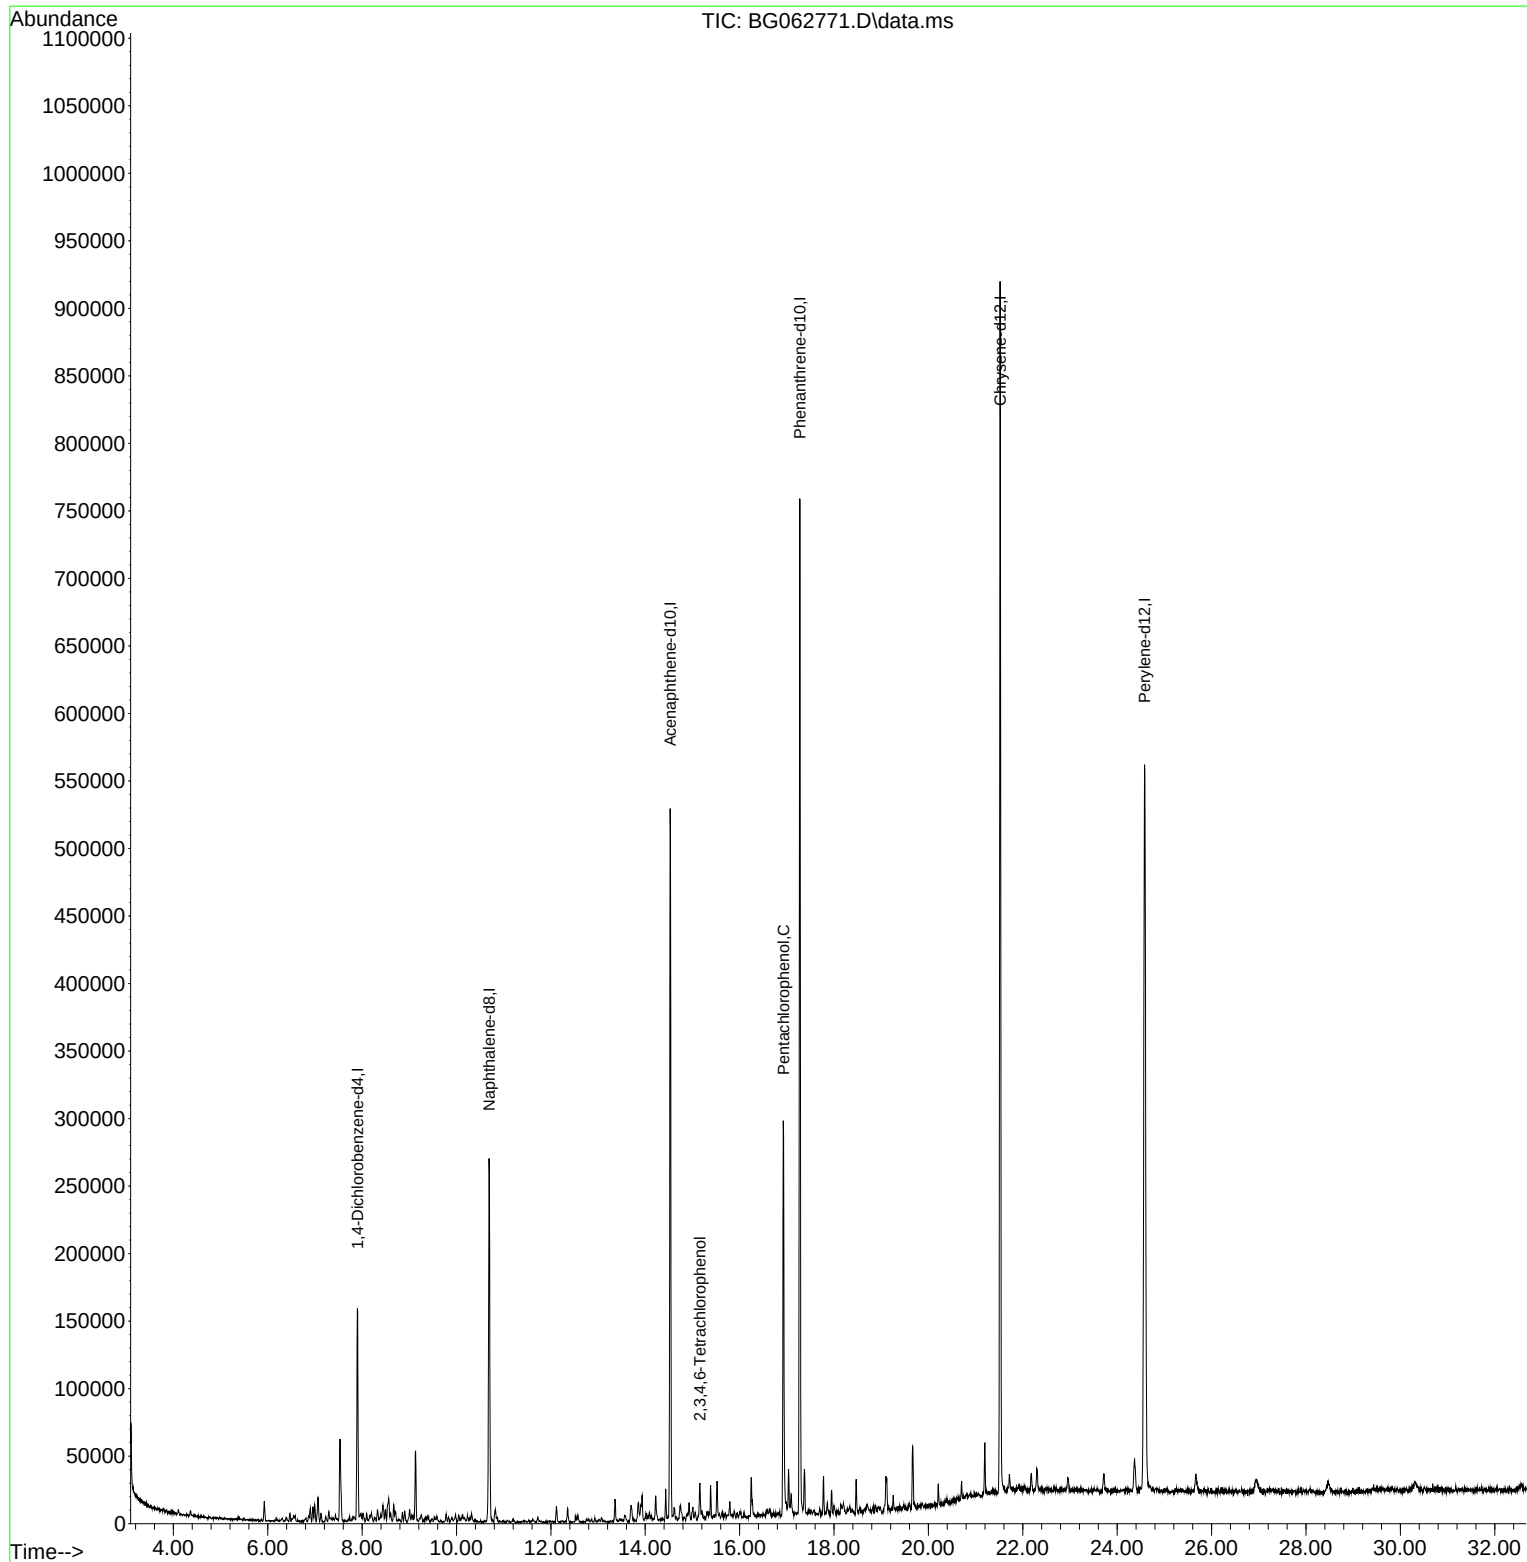


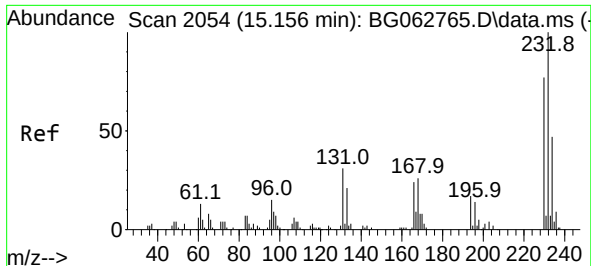

#58
2,3,4,6-Tetrachlorophenol
Concen: 1.278 ng/ul
RT: 15.156 min Scan# 2054
Delta R.T. 0.001 min
Lab File: BG062771.D
Acq: 12 Sep 2024 21:00

Instrument :
BNA_G
ClientSampleId :
DCVZ4DL

Tgt Ion:	232	Resp:	5684
Ion	Ratio	Lower	Upper
232	100		
131	33.3	26.6	40.0
130	0.0	1.6	2.4#
166	34.8	20.6	31.0#

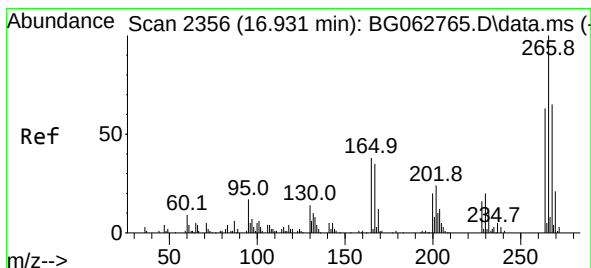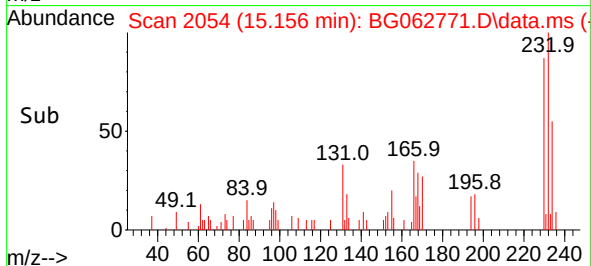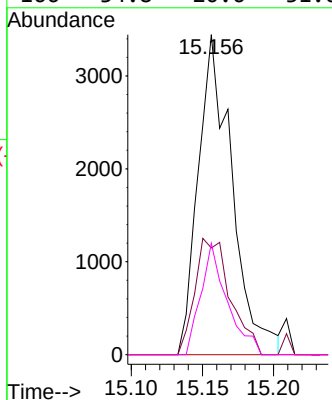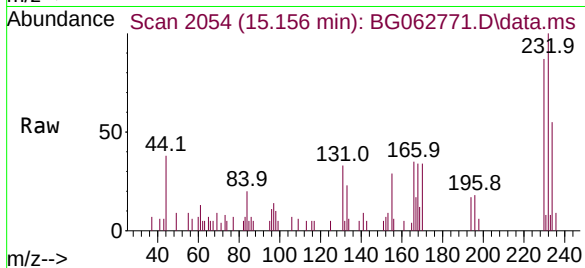

#71
Pentachlorophenol
Concen: 15.821 ng/ul
RT: 16.931 min Scan# 2356
Delta R.T. 0.001 min
Lab File: BG062771.D
Acq: 12 Sep 2024 21:00

Tgt Ion:	266	Resp:	63014
Ion	Ratio	Lower	Upper
266	100		
264	62.3	48.6	72.8
268	65.7	49.5	74.3

