

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
 Data File : BG062757.D
 Acq On : 12 Sep 2024 10:01
 Operator : JU/RC
 Sample : PB163311BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK311

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.194	16	18	22	rVB5	5242	6586	0.29%	0.034%
2	3.353	41	45	54	rVB2	14626	23606	1.03%	0.122%
3	3.758	110	114	132	rBV	163728	286763	12.52%	1.478%
4	4.240	194	196	202	rBV3	1957	2584	0.11%	0.013%
5	7.060	667	676	686	rBV	218719	363849	15.89%	1.875%
6	7.225	696	704	716	rBV	154714	258490	11.29%	1.332%
7	7.430	732	739	749	rBV	198408	336513	14.70%	1.735%
8	7.901	811	819	826	rBV	175127	291897	12.75%	1.505%
9	8.600	931	938	947	rBV	248085	412100	18.00%	2.124%
10	9.052	1006	1015	1028	rBV	181618	320576	14.00%	1.652%
11	9.775	1131	1138	1147	rBV	140086	250116	10.92%	1.289%
12	10.309	1221	1229	1239	rBV	245253	430662	18.81%	2.220%
13	10.691	1287	1294	1302	rVB	253504	439889	19.21%	2.267%
14	10.821	1305	1316	1329	rBV	226196	411198	17.96%	2.120%
15	12.284	1560	1565	1570	rBV3	3920	6121	0.27%	0.032%
16	13.935	1839	1846	1854	rVB	551468	805004	35.16%	4.149%
17	14.222	1888	1895	1905	rBV	651601	999921	43.67%	5.154%
18	14.528	1941	1947	1957	rVB	531455	831980	36.34%	4.289%
19	14.722	1974	1980	1990	rBV	247742	407804	17.81%	2.102%
20	15.345	2080	2086	2090	rBV2	1485	3699	0.16%	0.019%
21	15.521	2110	2116	2125	rBV	921618	1366655	59.69%	7.045%
22	15.638	2130	2136	2146	rBV	247910	377503	16.49%	1.946%
23	15.756	2154	2156	2162	rVB4	3324	4794	0.21%	0.025%
24	16.314	2245	2251	2253	rBV4	3363	5756	0.25%	0.030%
25	17.278	2407	2415	2425	rBV	792683	1190955	52.01%	6.139%
26	17.378	2425	2432	2440	rBV2	1093031	1695787	74.06%	8.741%
27	17.942	2522	2528	2529	rBV3	1884	2687	0.12%	0.014%
28	18.235	2577	2578	2582	rBV3	2410	2500	0.11%	0.013%
29	18.488	2617	2621	2626	rBV4	1853	4154	0.18%	0.021%
30	19.228	2744	2747	2753	rBV3	15219	22210	0.97%	0.114%
31	19.299	2755	2759	2767	rVB3	14401	22155	0.97%	0.114%
32	19.364	2767	2770	2773	rBV3	1641	2498	0.11%	0.013%
33	19.575	2802	2806	2807	rBV3	2999	3452	0.15%	0.018%
34	19.593	2807	2809	2815	rVV4	2448	4073	0.18%	0.021%
35	19.663	2815	2821	2830	rBV	1515447	2192470	95.75%	11.301%
36	19.834	2848	2850	2853	rBV2	1927	2455	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
 Data File : BG062757.D
 Acq On : 12 Sep 2024 10:01
 Operator : JU/RC
 Sample : PB163311BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK311

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	19.963	2871	2872	2875	rBV3	3421	3072	0.13%	0.016%
38	20.016	2879	2881	2884	rBV3	2099	2814	0.12%	0.015%
39	20.298	2927	2929	2933	rBV4	2770	3513	0.15%	0.018%
40	20.386	2940	2944	2945	rBV2	2896	3376	0.15%	0.017%
41	20.639	2984	2987	2991	rBV6	5596	8377	0.37%	0.043%
42	21.126	3064	3070	3071	rBV4	11474	17297	0.76%	0.089%
43	21.197	3078	3082	3086	rBV7	8790	18227	0.80%	0.094%
44	21.255	3091	3092	3093	rBV	5389	2411	0.11%	0.012%
45	21.520	3131	3137	3148	rBV2	922541	1483142	64.78%	7.645%
46	21.720	3169	3171	3175	rVB5	7093	9410	0.41%	0.049%
47	21.949	3207	3210	3212	rBV3	4574	6064	0.26%	0.031%
48	22.301	3265	3270	3275	rBV7	9606	21985	0.96%	0.113%
49	22.413	3287	3289	3290	rBV2	4036	2745	0.12%	0.014%
50	22.830	3358	3360	3362	rBV3	4454	2820	0.12%	0.015%
51	22.865	3364	3366	3370	rBV5	3490	4360	0.19%	0.022%
52	22.953	3378	3381	3386	rBV7	11576	20634	0.90%	0.106%
53	23.723	3506	3512	3517	rVB4	17960	34842	1.52%	0.180%
54	24.287	3607	3608	3611	rBV2	4802	2954	0.13%	0.015%
55	24.375	3611	3623	3635	rBV2	884594	2289667	100.00%	11.802%
56	24.587	3648	3659	3672	rBV	569541	1592028	69.53%	8.206%
57	25.674	3839	3844	3851	rVB7	18381	43466	1.90%	0.224%
58	26.796	4033	4035	4036	rVB2	5601	2604	0.11%	0.013%
59	26.937	4057	4059	4060	rBV	7674	6171	0.27%	0.032%
60	28.106	4256	4258	4262	rVB5	5314	3842	0.17%	0.020%
61	29.863	4555	4557	4560	rVB4	4492	3789	0.17%	0.020%
62	29.986	4575	4578	4580	rBV4	6036	7302	0.32%	0.038%
63	30.844	4722	4724	4729	rBV6	3590	4943	0.22%	0.025%
64	31.191	4781	4783	4785	rBV3	5062	2986	0.13%	0.015%
65	31.379	4813	4815	4816	rBV2	3973	2567	0.11%	0.013%
66	31.908	4903	4905	4908	rBV4	3522	3271	0.14%	0.017%




Sum of corrected areas: 19400141

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
Data File : BG062757.D
Acq On : 12 Sep 2024 10:01
Operator : JU/RC
Sample : PB163311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK311

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

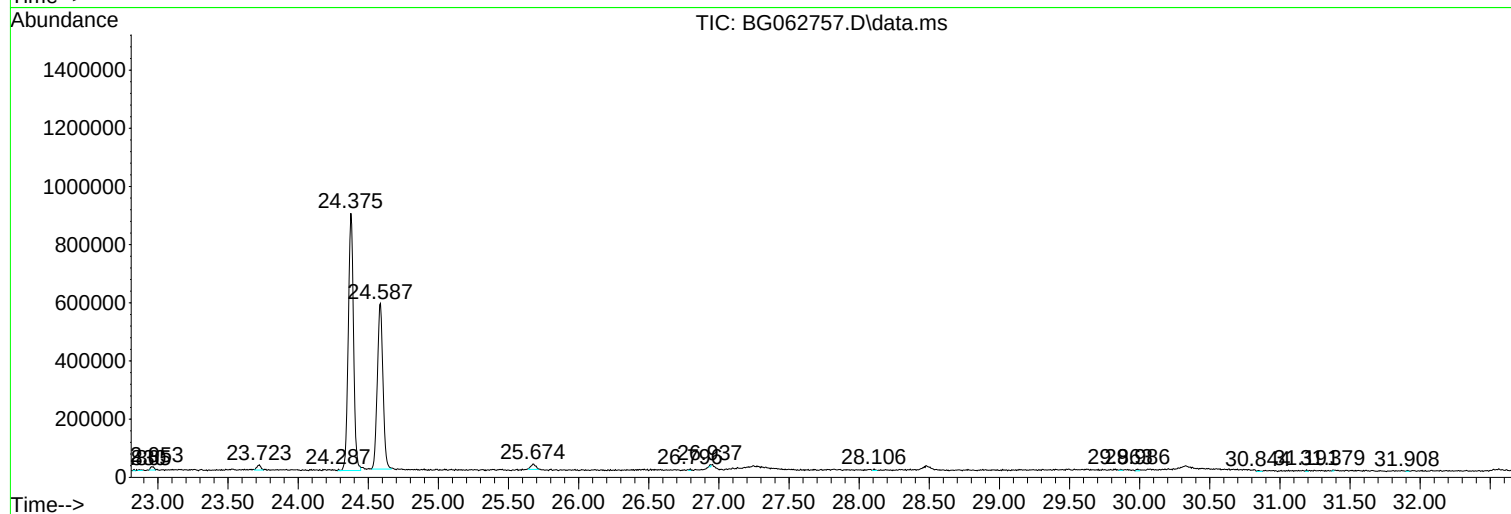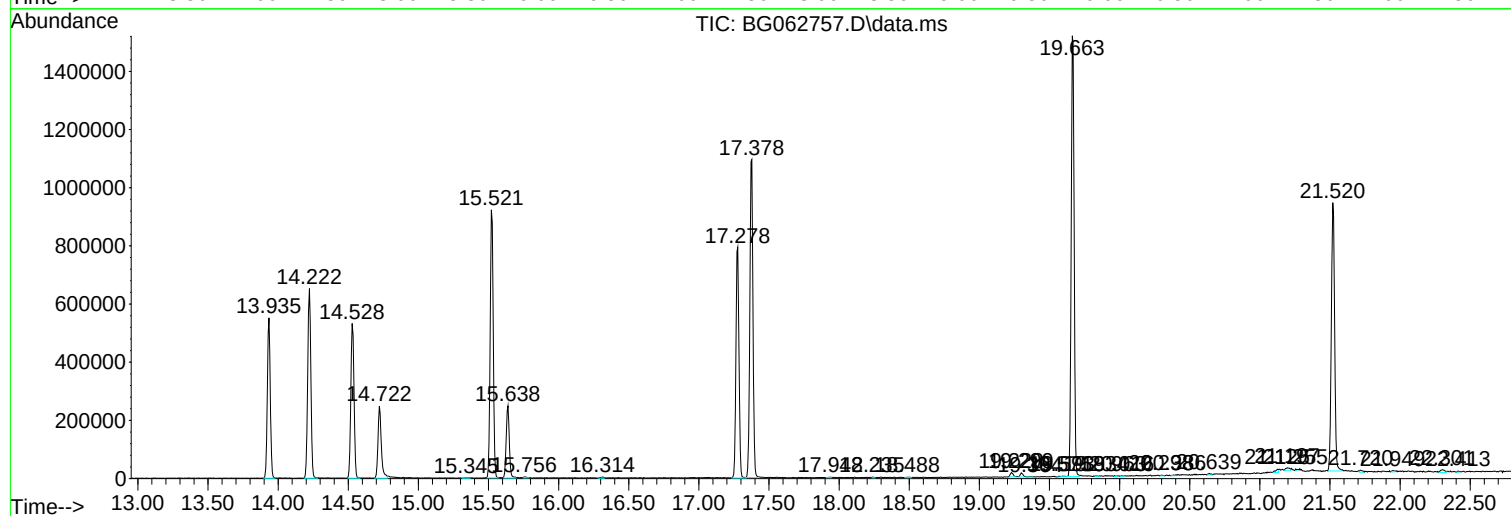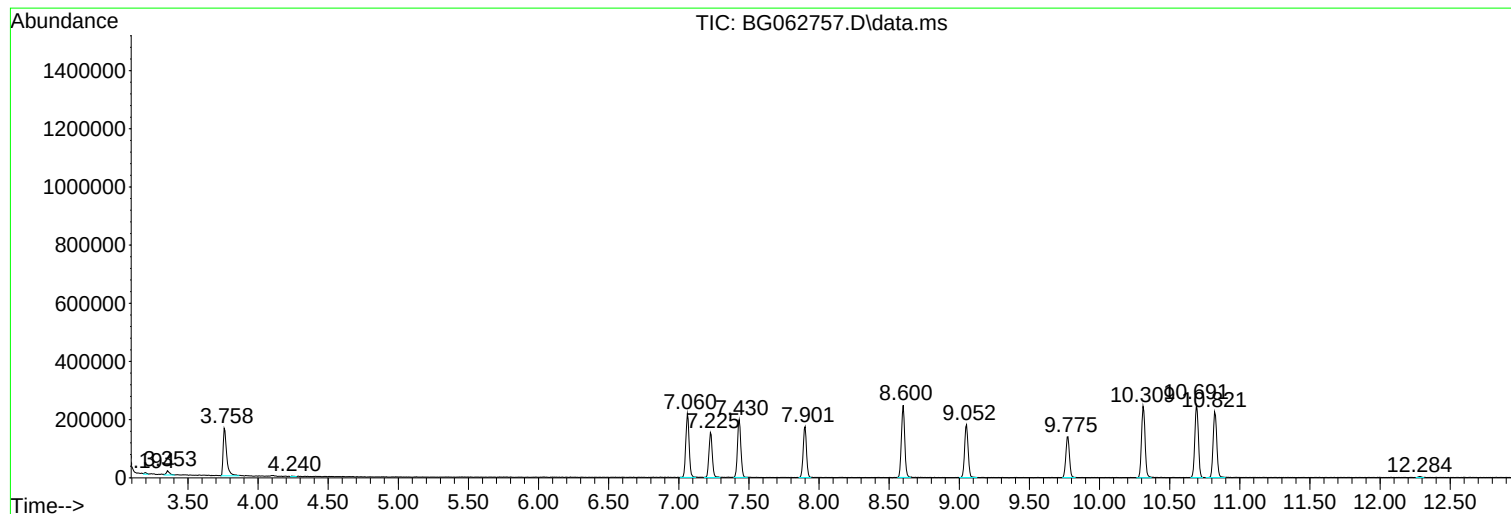

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
Data File : BG062757.D
Acq On : 12 Sep 2024 10:01
Operator : JU/RC
Sample : PB163311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK311

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091224\
Data File : BG062757.D
Acq On : 12 Sep 2024 10:01
Operator : JU/RC
Sample : PB163311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK311

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc