


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091225\
Data File : BG064353.D
Acq On : 12 Sep 2025 10:34
Operator : RC/JU
Sample : DFTPP457
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP457

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Title : SVOA CALIBRATION
Last Update : Fri Sep 12 11:06:20 2025

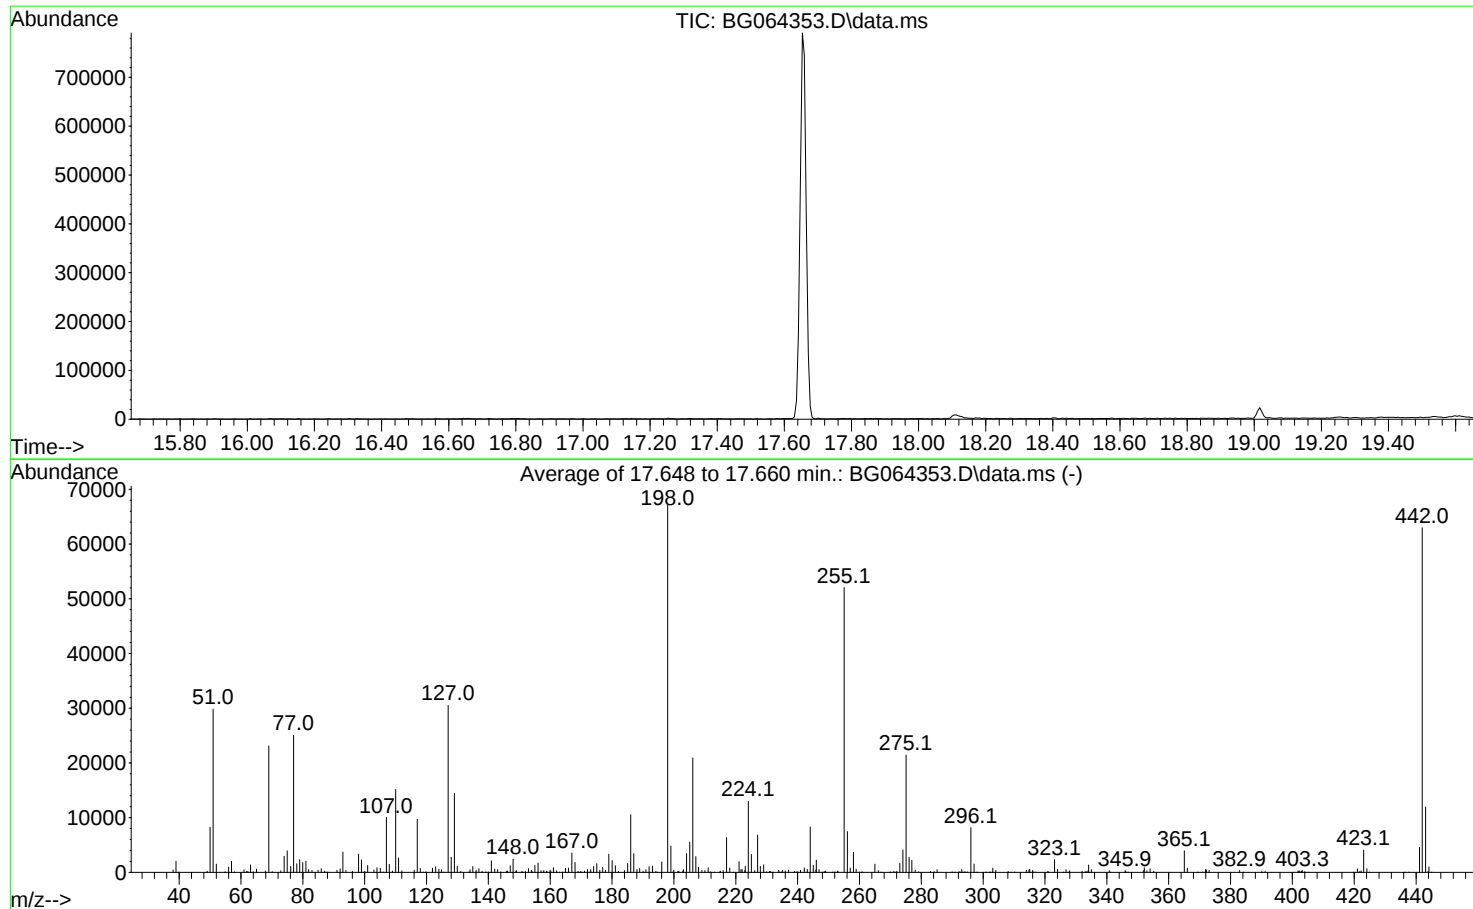

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	29837	PASS
68	69	0.00	2	1.2	267	PASS
69	198	0.00	100	34.4	23112	PASS
70	69	0.00	2	0.7	162	PASS
127	198	10	80	45.4	30528	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67221	PASS
199	198	5	9	7.1	4785	PASS
275	198	10	60	31.9	21429	PASS
365	198	1	100	5.9	3939	PASS
441	198	0.01	100	6.8	4603	PASS
442	198	50	100	93.7	62992	PASS
443	442	15	24	19.0	11974	PASS