
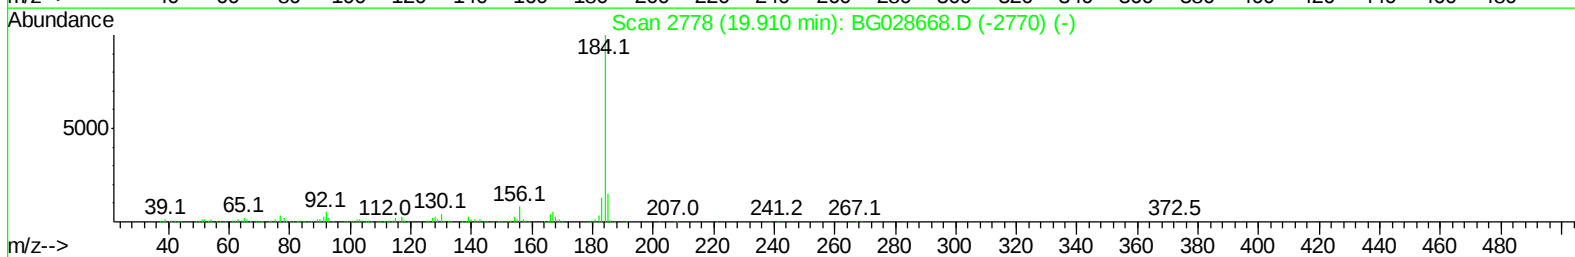
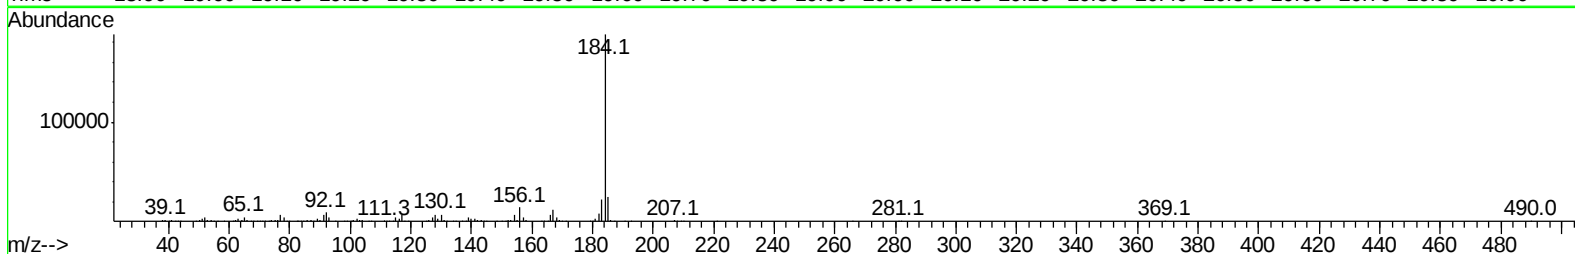


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
Data File : BG028691.D
Acq On : 13 Sep 2017 10:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 09:31:51 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

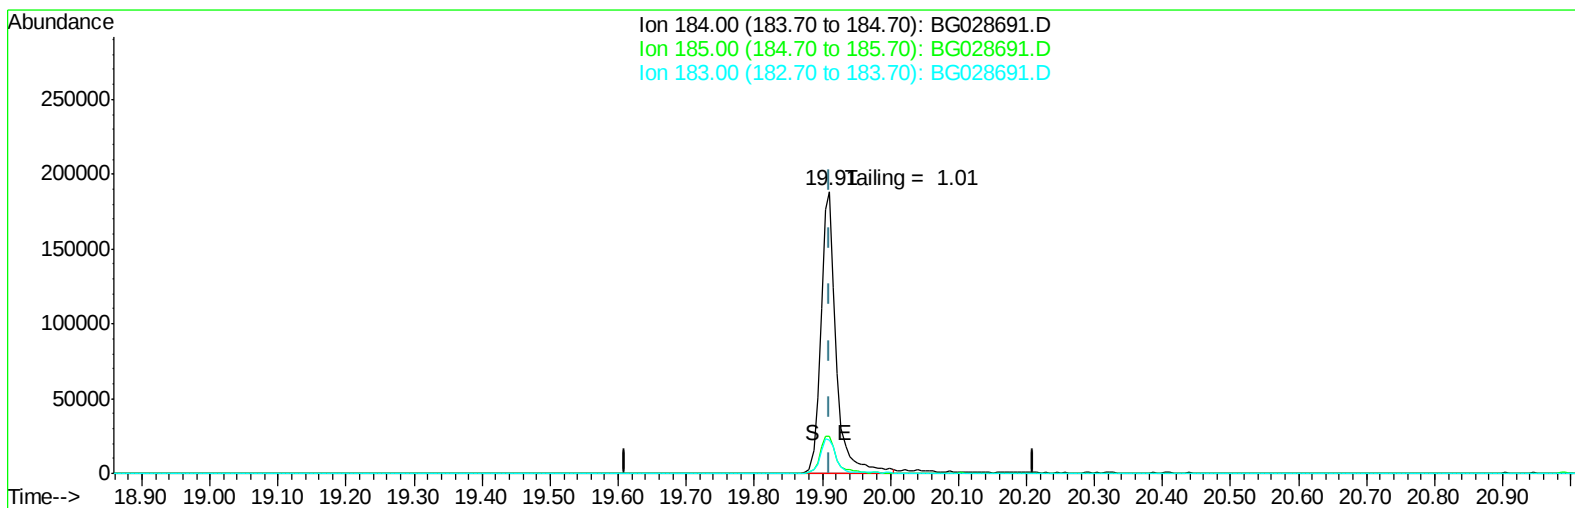

TIC: BG028691.D

(76) Benzidine




19.910min (-0.000) 0.00ng

response 299520

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.03#
183.00	13.80	11.91
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
Data File : BG028691.D
Acq On : 13 Sep 2017 10:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 09:31:51 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

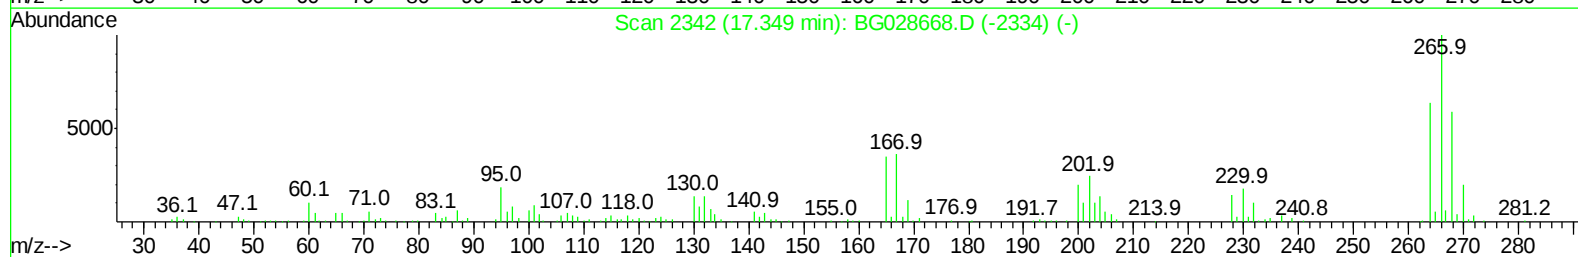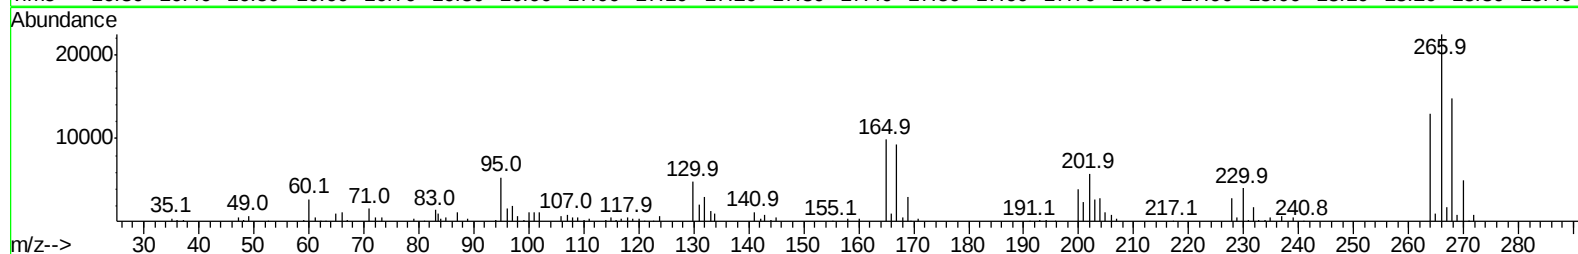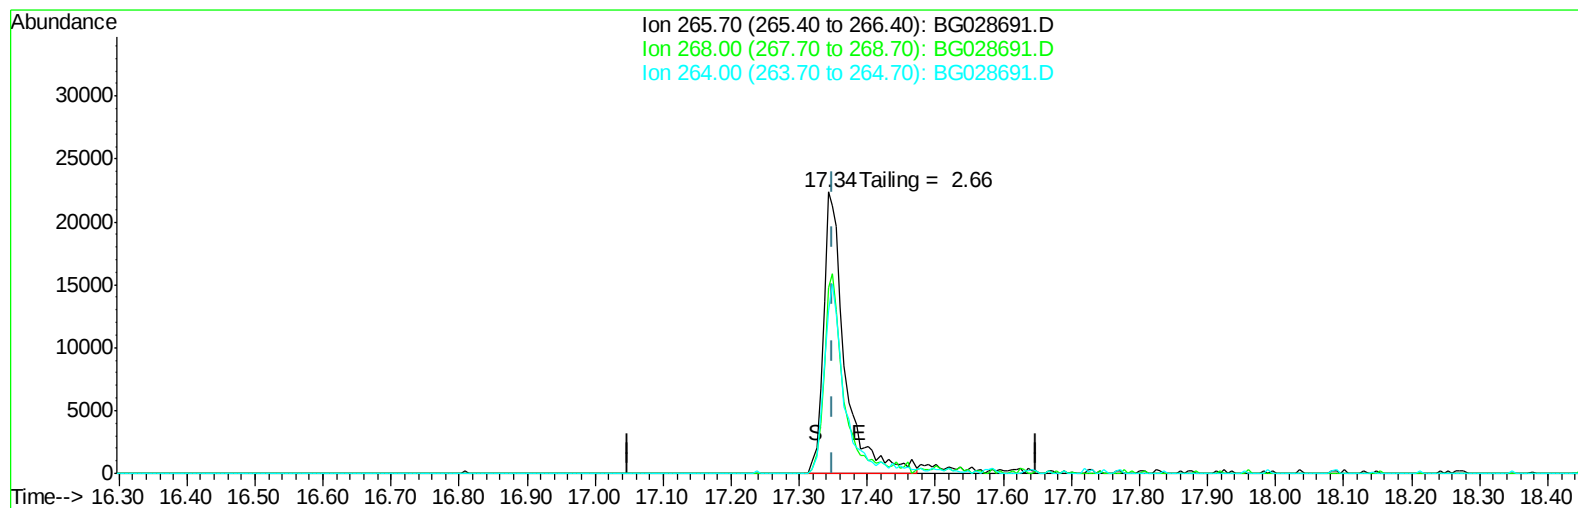

TIC: BG028691.D

(69) Pentachlorophenol (C)

17.343min (-0.006) 117988.01ng

response 48404

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	65.77
264.00	62.60	57.89
0.00	0.00	0.00