
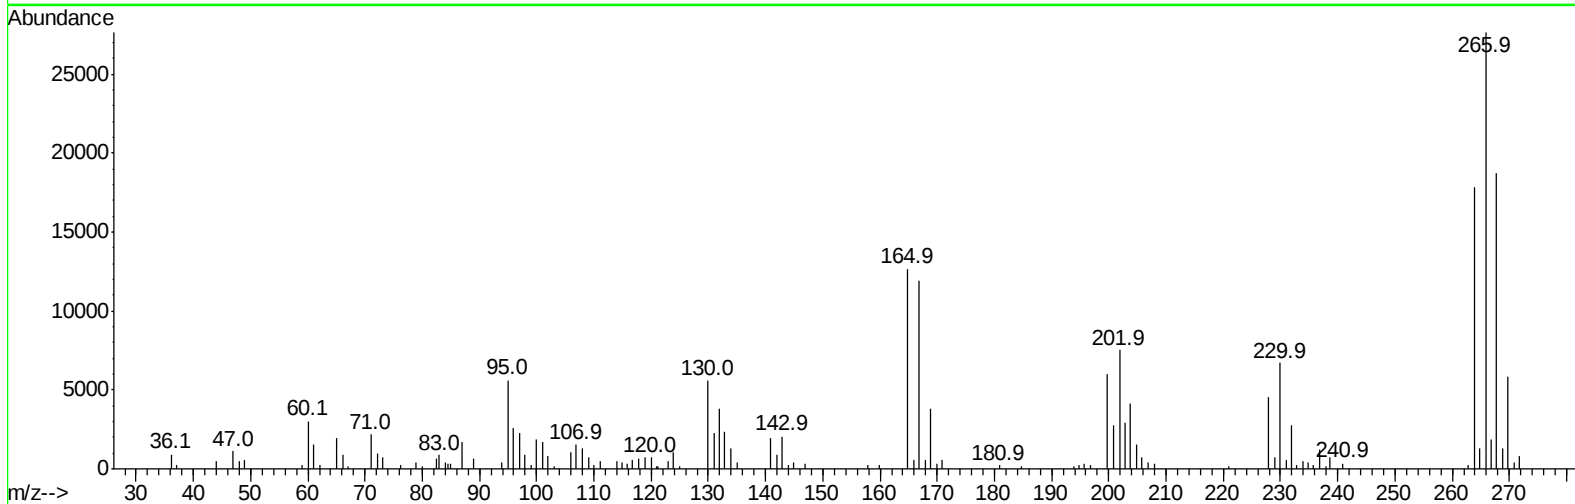


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
Data File : BG028710.D
Acq On : 13 Sep 2017 22:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 09:32:54 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

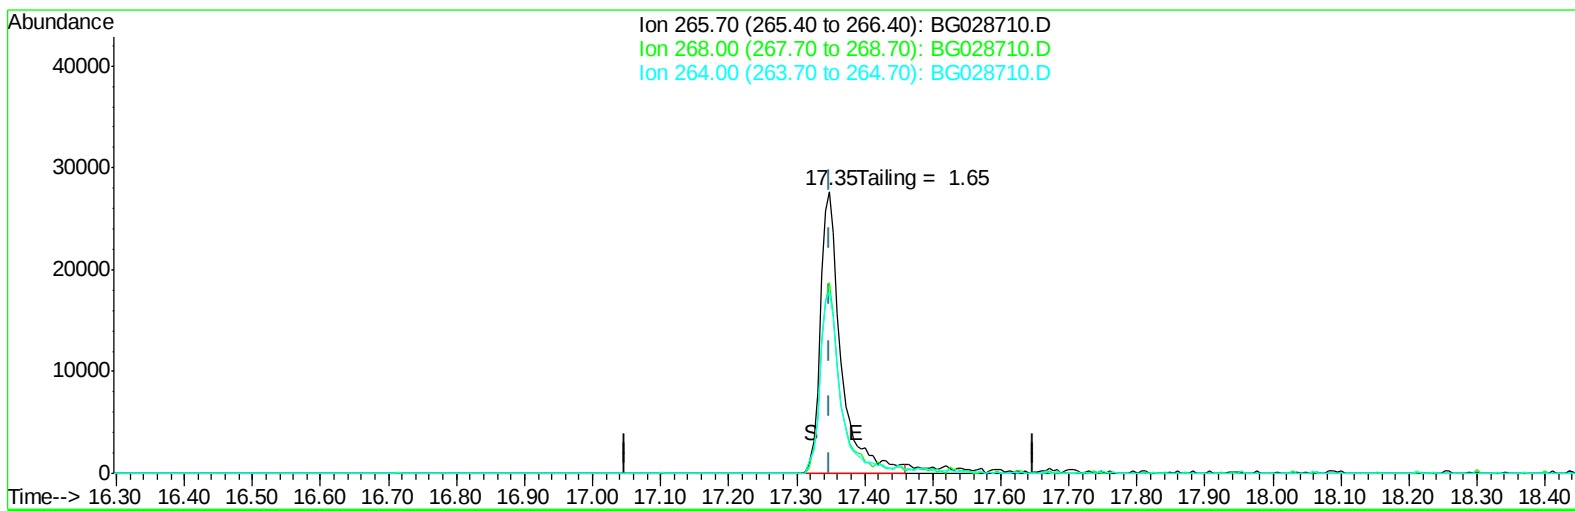

TIC: BG028710.D

(69) Pentachlorophenol (C)



17.348min (-0.001) 0.00ng

response 58911

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	67.62
264.00	62.60	69.03
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
Data File : BG028710.D
Acq On : 13 Sep 2017 22:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 09:32:54 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

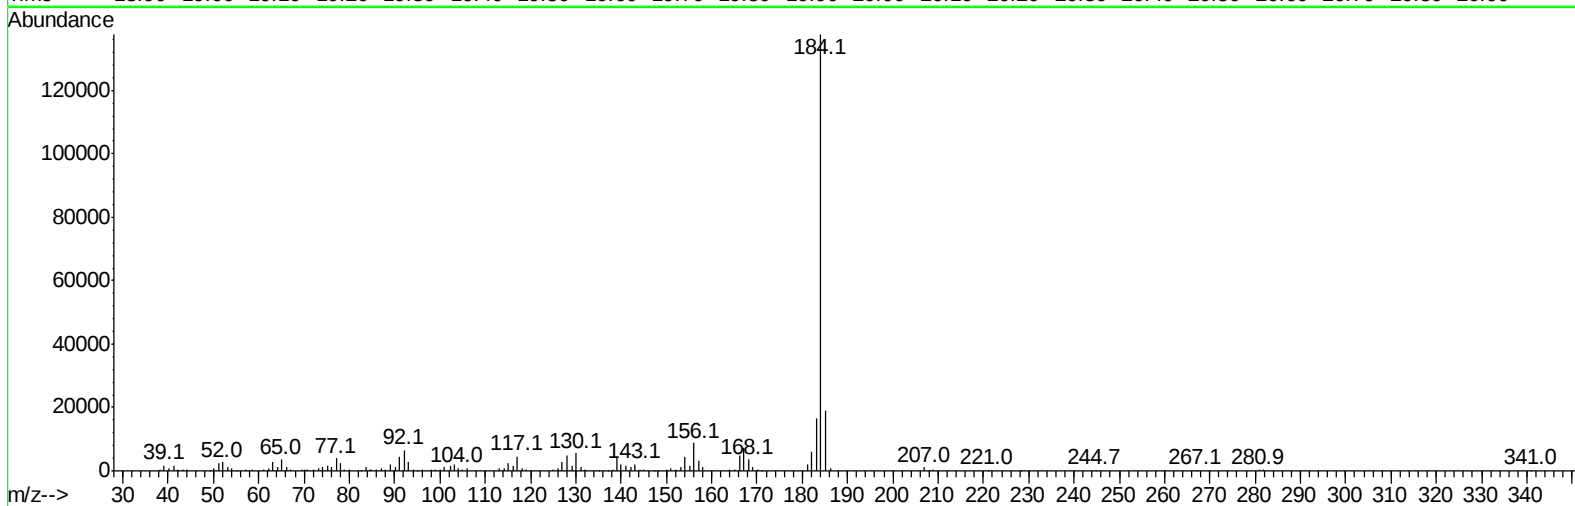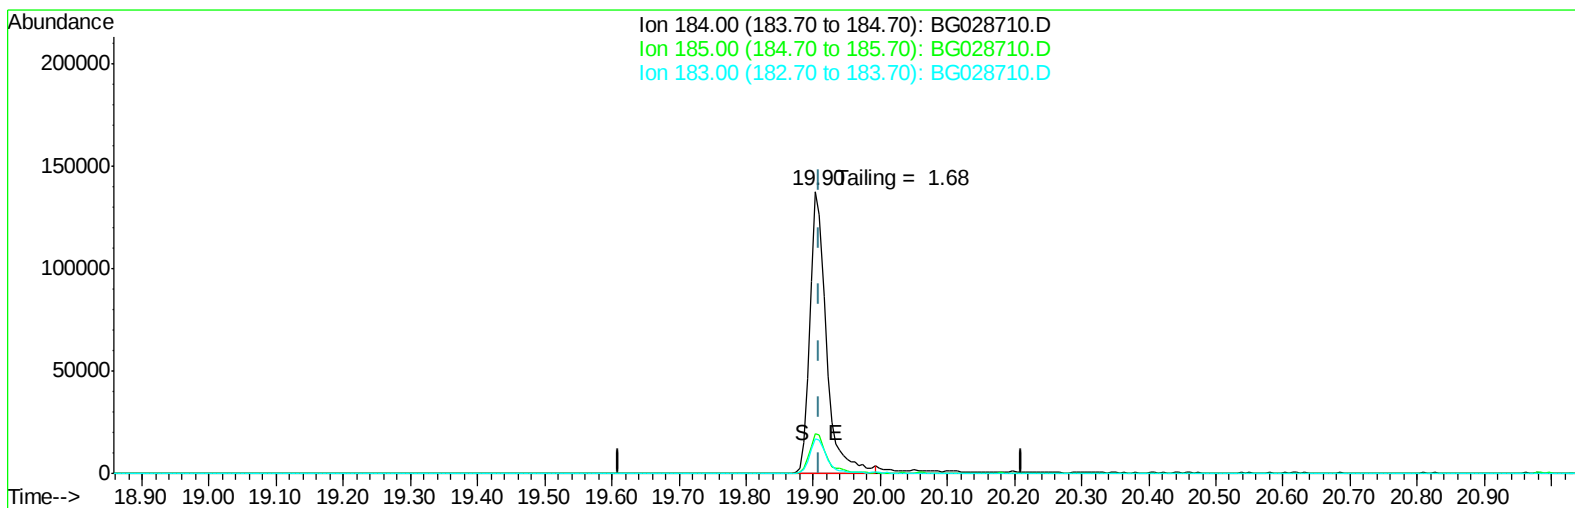

TIC: BG028710.D

(76) Benzidine

19.904min (-0.007) 115915.07ng

response 234464

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.89
183.00	13.80	12.08
0.00	0.00	0.00