

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
 Data File : BG028698.D
 Acq On : 13 Sep 2017 14:48
 Operator : SJ/JU
 Sample : I5189-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C-MW-07-090717

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.900	385	393	402	rBV	238910	415312	11.25%	3.320%
2	7.481	653	662	673	rBV	132211	260735	7.06%	2.084%
3	7.863	720	727	743	rVB	443307	792190	21.46%	6.332%
4	8.327	800	806	815	rVB	90384	157349	4.26%	1.258%
5	8.656	852	862	870	rBV	393054	723112	19.59%	5.780%
6	9.496	997	1005	1018	rBV	328623	643359	17.43%	5.143%
7	11.147	1278	1286	1293	rBV	112726	217660	5.90%	1.740%
8	13.562	1689	1697	1711	rBV	1029336	1661544	45.01%	13.281%
9	14.937	1924	1931	1941	rBV2	198879	350489	9.49%	2.802%
10	16.429	2178	2185	2198	rBV	1091003	1704895	46.18%	13.628%
11	17.692	2393	2400	2411	rBV2	350872	551352	14.93%	4.407%
12	20.278	2834	2840	2851	rBV	2855118	3691713	100.00%	29.509%
13	22.023	3130	3137	3149	rVB	405013	702086	19.02%	5.612%
14	25.524	3721	3733	3744	rVB2	204282	638592	17.30%	5.104%


Sum of corrected areas: 12510388

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
Data File : BG028698.D
Acq On : 13 Sep 2017 14:48
Operator : SJ/JU
Sample : I5189-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C-MW-07-090717

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

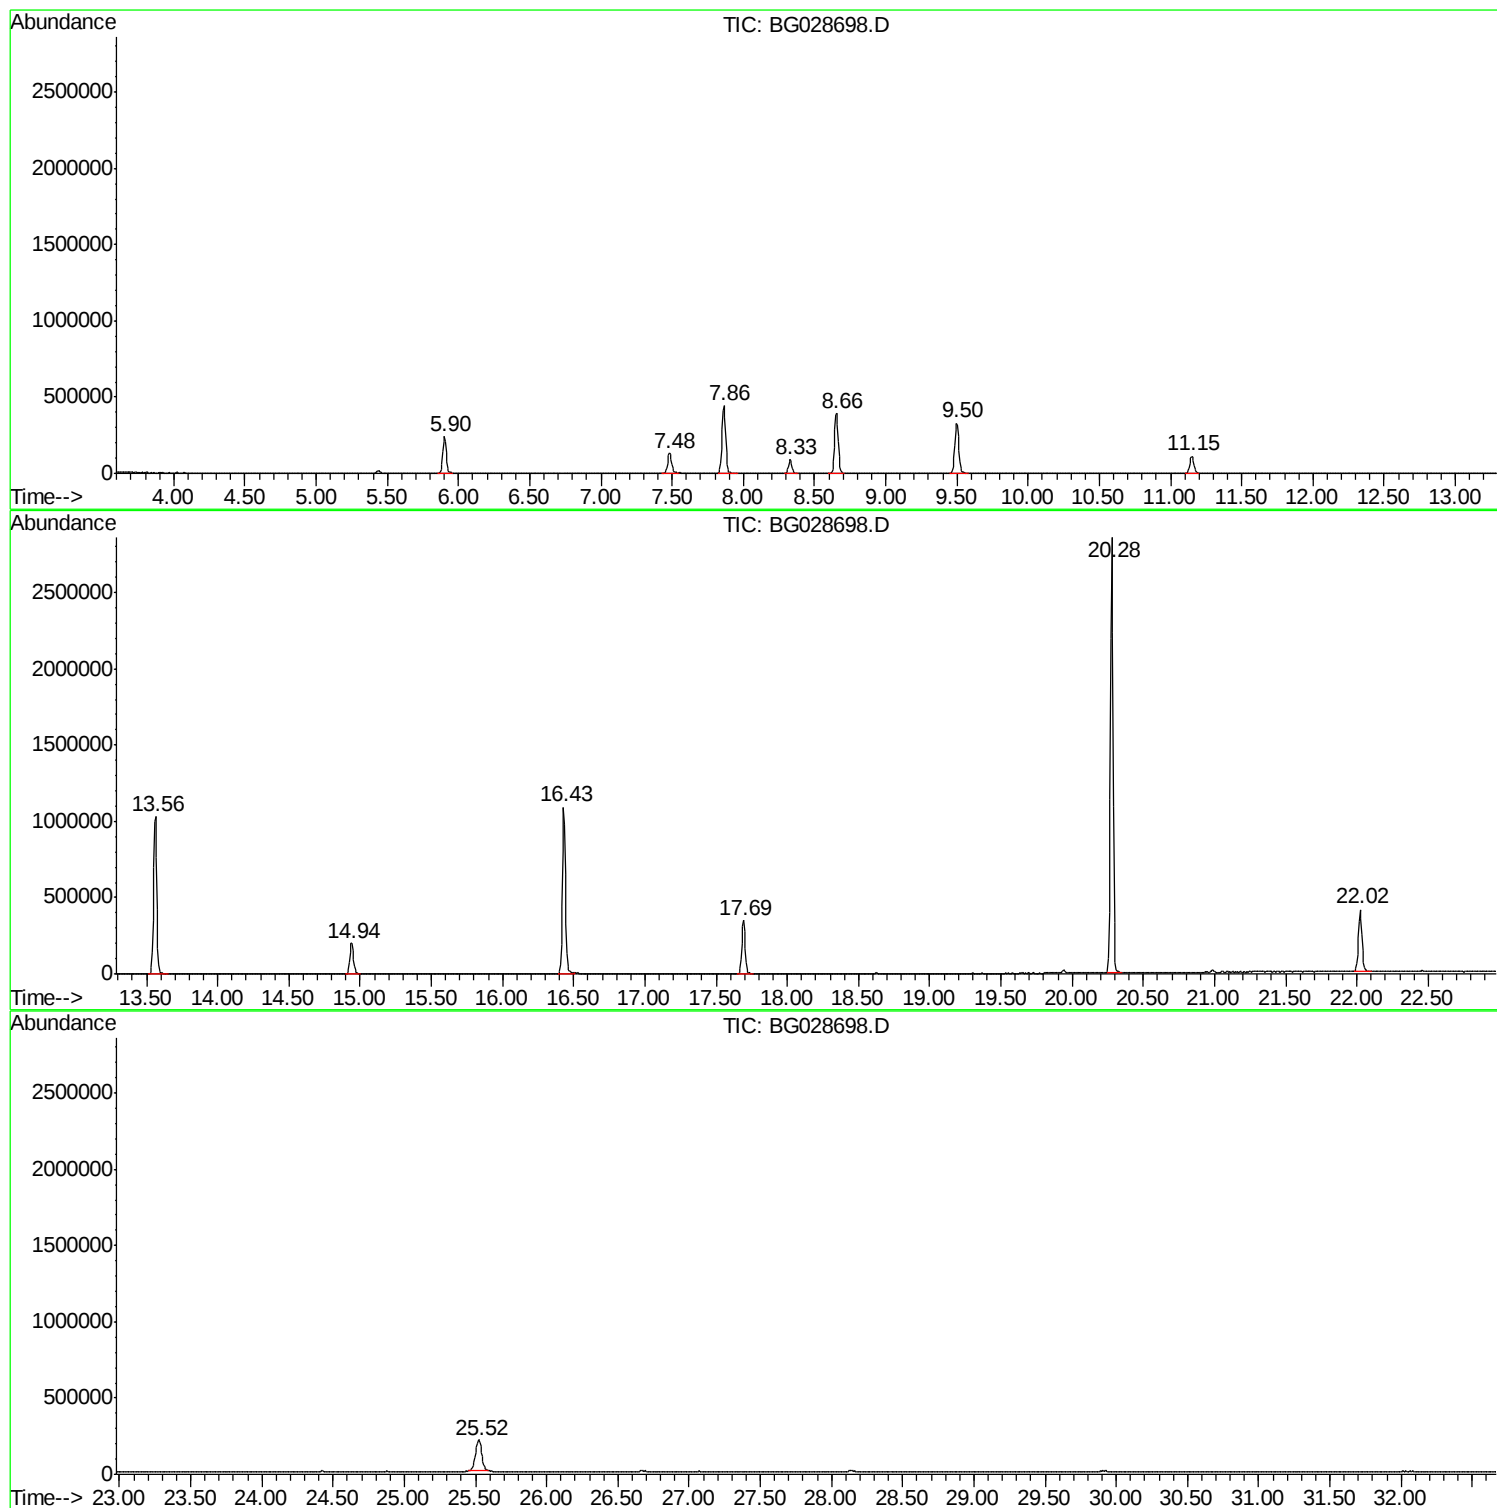

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG091317\
Data File : BG028698.D
Acq On : 13 Sep 2017 14:48
Operator : SJ/JU
Sample : I5189-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C-MW-07-090717










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.86 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.86	100.69 ng	792190	1,4-Dichlorobenzene-d4	8.33

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10

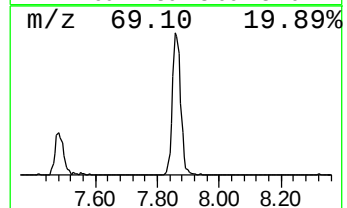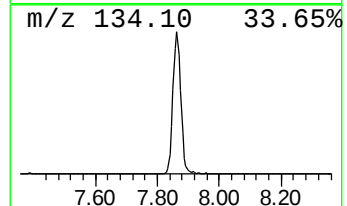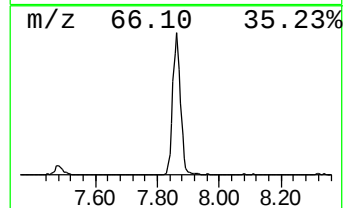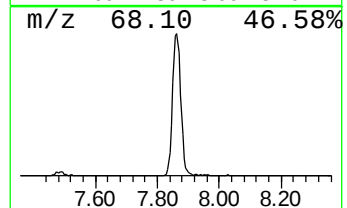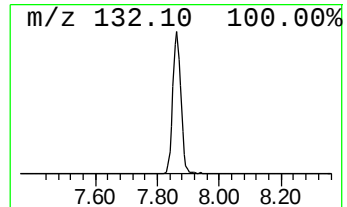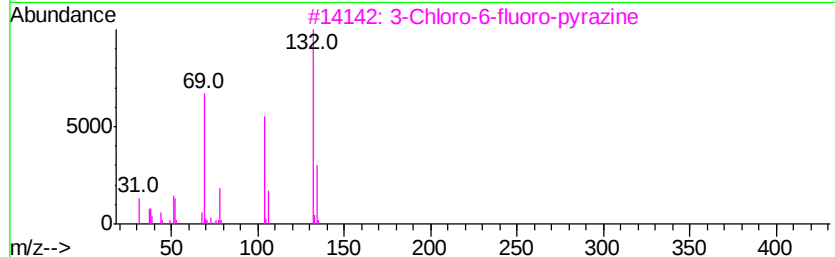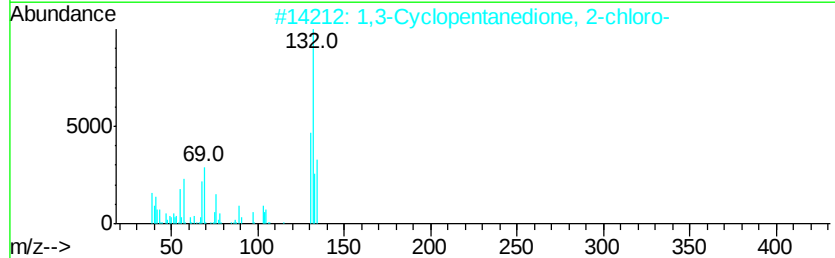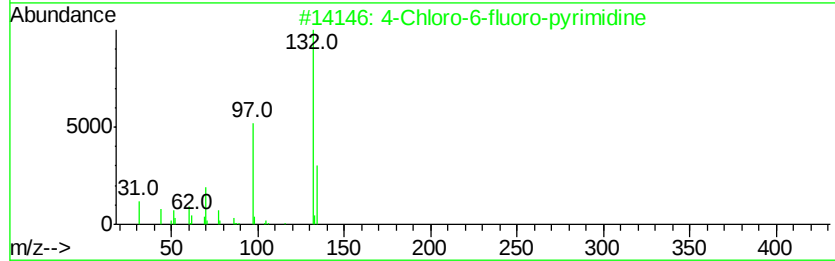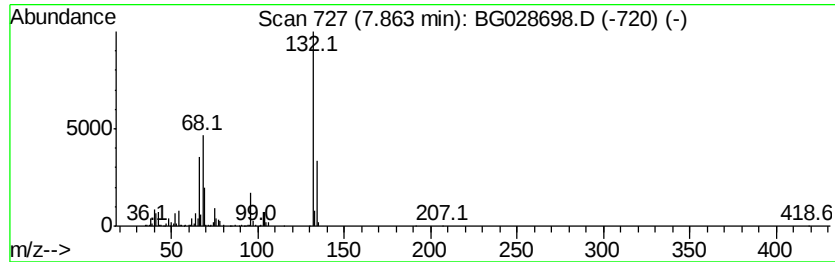

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG091317\
Data File : BG028698.D
Acq On : 13 Sep 2017 14:48
Operator : SJ/JU
Sample : I5189-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C-MW-07-090717

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.86	7.86	100.7	ng	792190	1	8.33	157349	20.0