


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
 Data File : BG028691.D
 Acq On : 13 Sep 2017 10:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

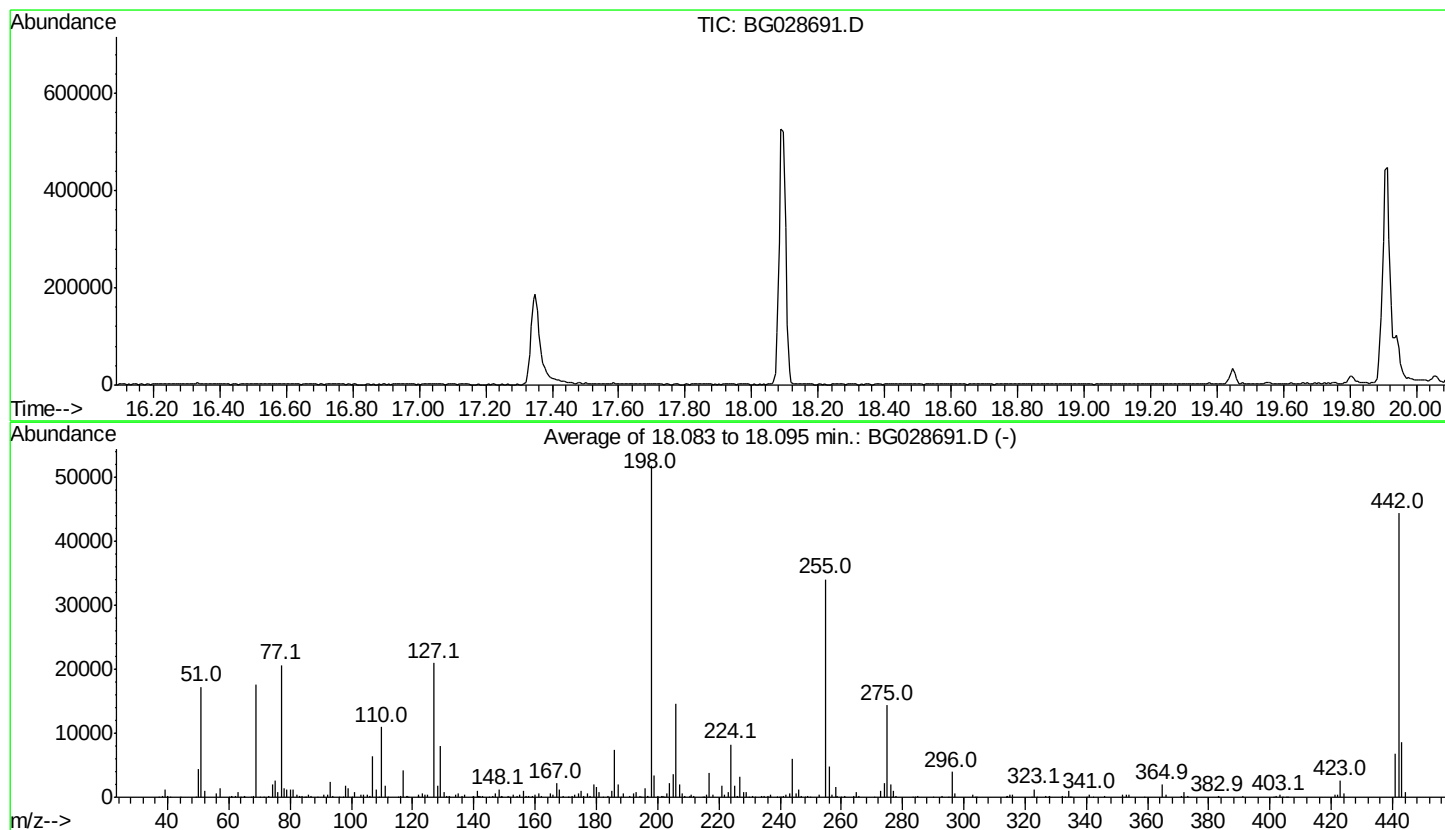

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	17264	PASS
68	69	0.00	2	1.2	211	PASS
69	198	0.00	100	33.9	17581	PASS
70	69	0.00	2	0.4	78	PASS
127	198	10	80	40.5	21004	PASS
197	198	0.00	2	0.3	172	PASS
198	198	100	100	100.0	51888	PASS
199	198	5	9	6.7	3501	PASS
275	198	10	60	27.7	14382	PASS
365	198	1	100	3.8	1952	PASS
441	442	0.01	24	15.2	6737	PASS
442	198	50	100	85.6	44432	PASS
443	442	15	24	19.3	8571	PASS