


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091317\
 Data File : BG028710.D
 Acq On : 13 Sep 2017 23:23
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

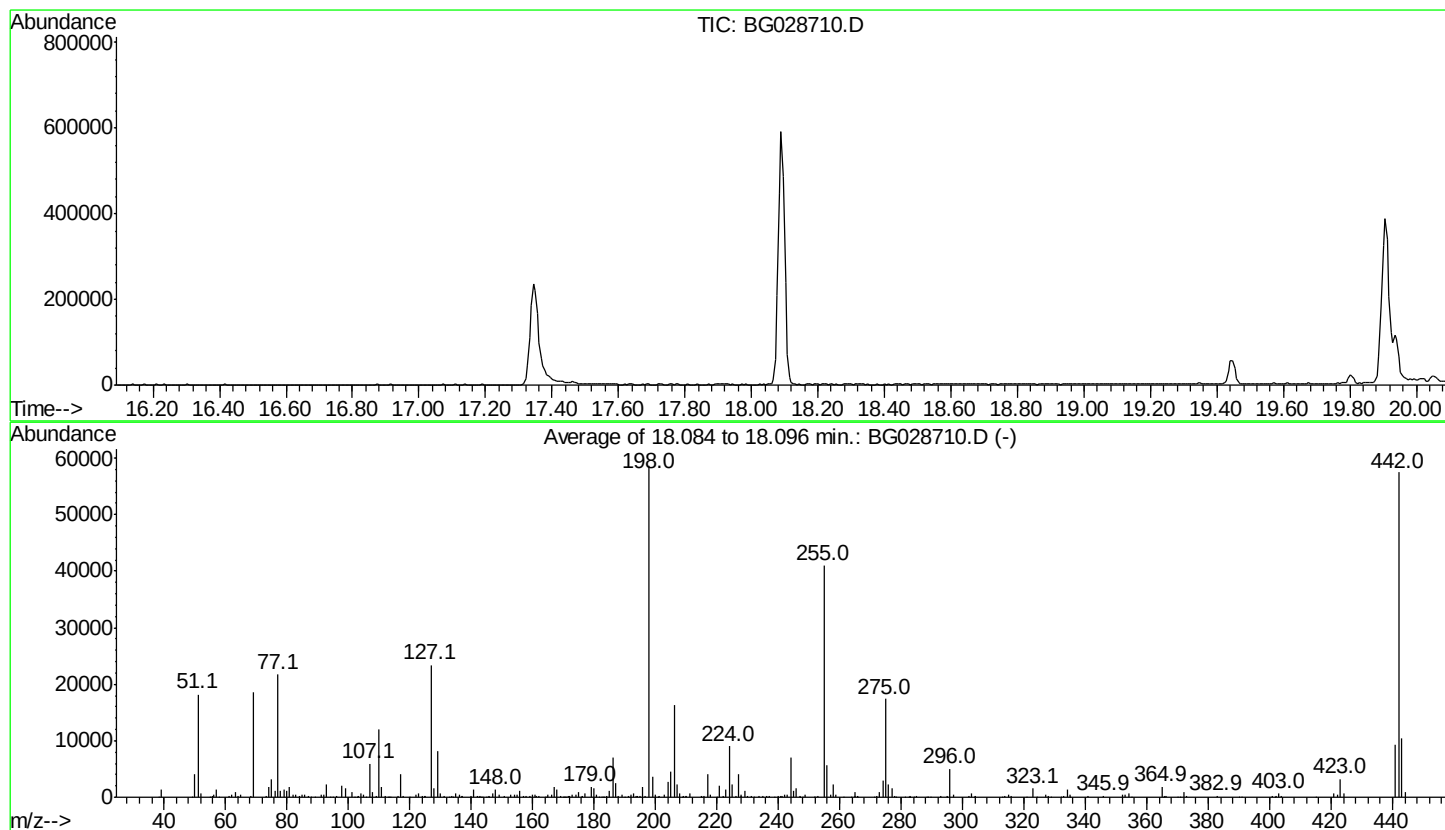

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	18198	PASS
68	69	0.00	2	0.9	169	PASS
69	198	0.00	100	31.8	18672	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.8	23360	PASS
197	198	0.00	2	0.4	248	PASS
198	198	100	100	100.0	58685	PASS
199	198	5	9	6.2	3652	PASS
275	198	10	60	29.7	17405	PASS
365	198	1	100	3.2	1873	PASS
441	442	0.01	24	16.3	9381	PASS
442	198	50	100	98.2	57605	PASS
443	442	15	24	18.0	10381	PASS