
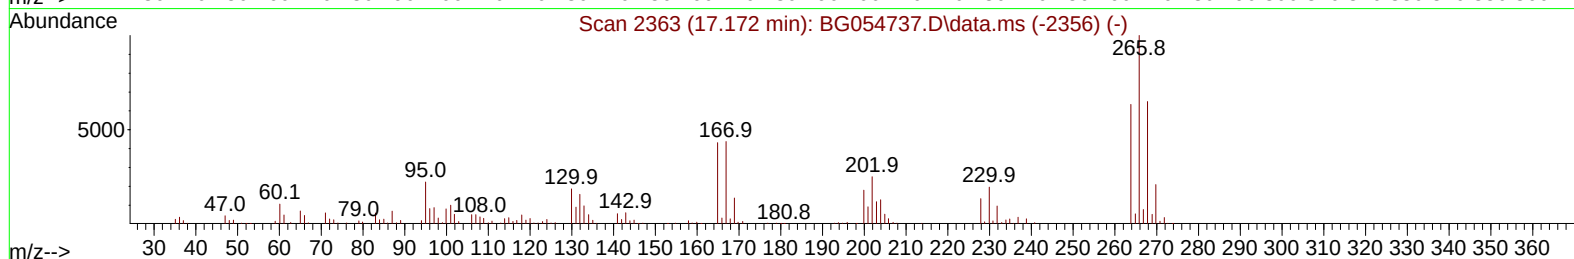
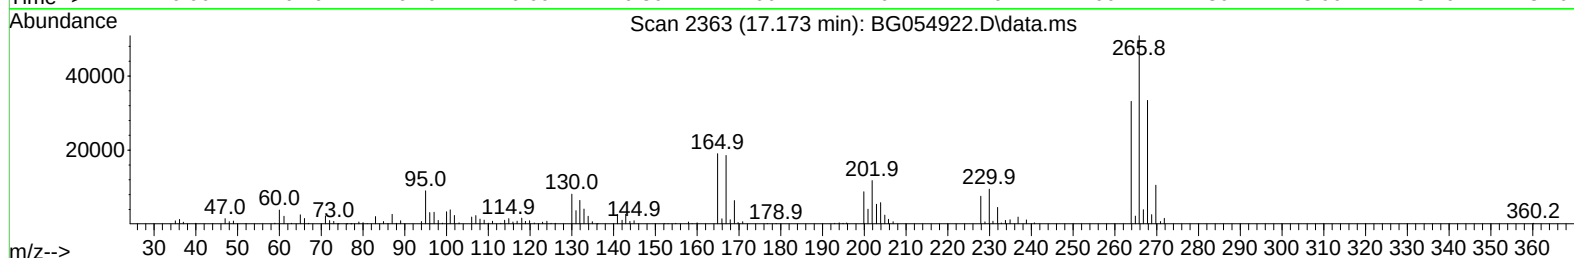


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
Data File : BG054922.D
Acq On : 13 Sep 2022 13:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 14:36:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

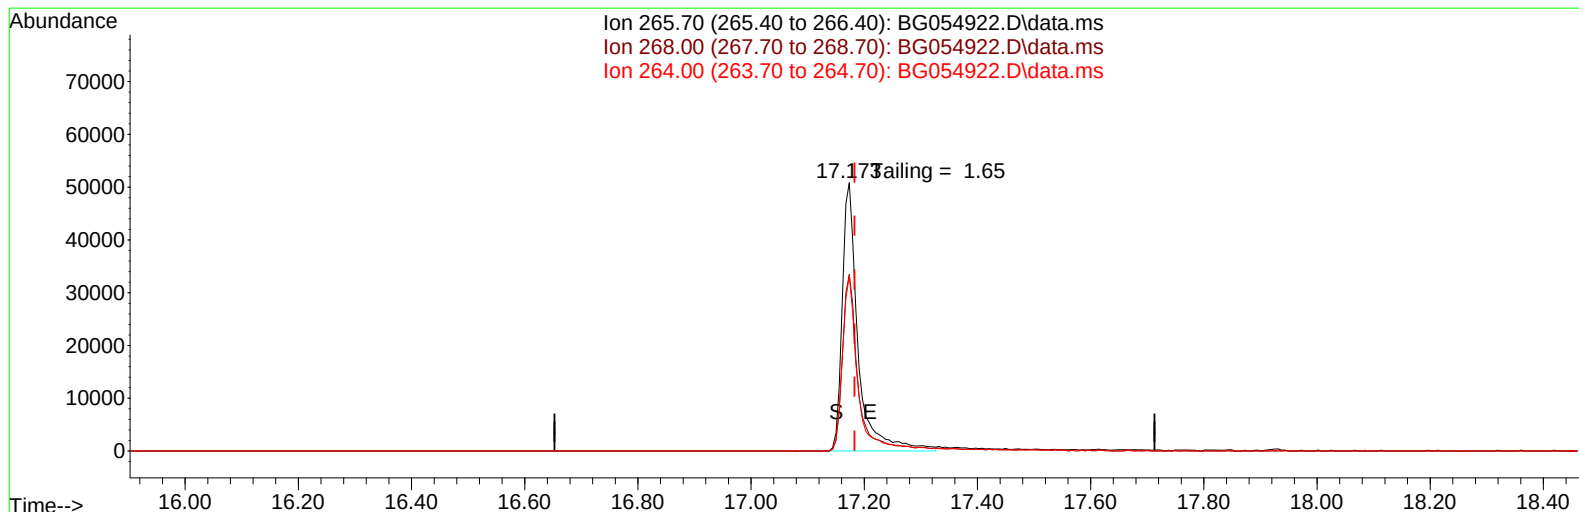

TIC: BG054922.D\data.ms

(70) Pentachlorophenol (C)




17.173min (-0.009) 38414.62 ng

response 99438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.75
264.00	61.70	65.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
Data File : BG054922.D
Acq On : 13 Sep 2022 13:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 14:36:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

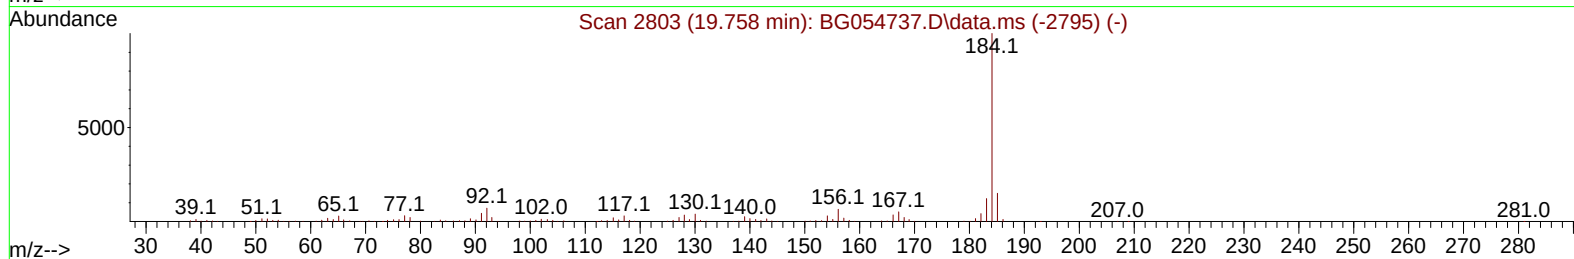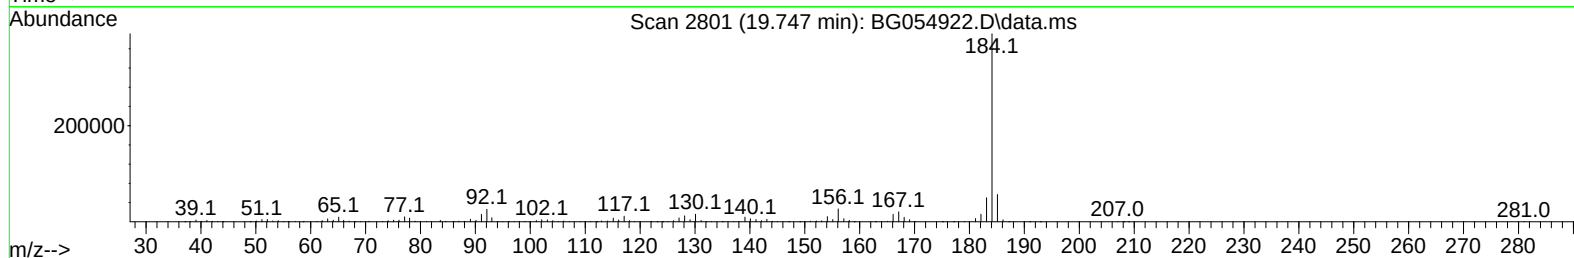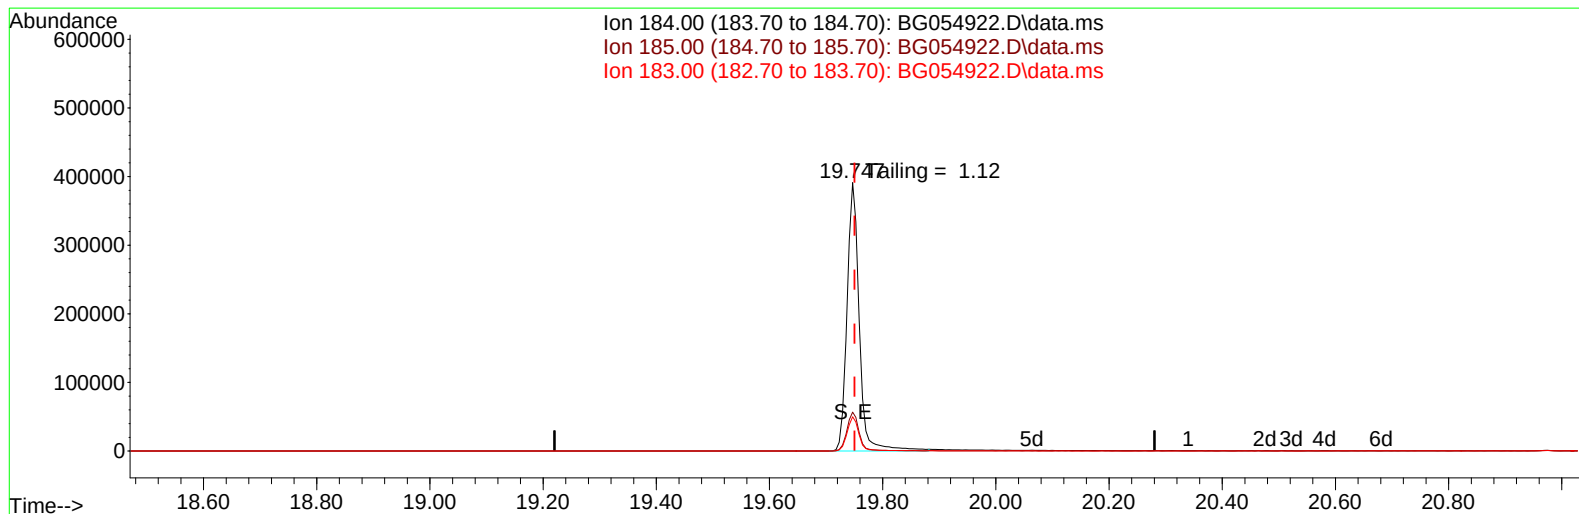

TIC: BG054922.D\data.ms

(77) Benzidine

19.747min (-0.003) 447789.20 ng m

response 587833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.51
183.00	12.30	12.78
0.00	0.00	0.00