

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
 Data File : BG054937.D
 Acq On : 14 Sep 2022 1:19
 Operator : CG/JU
 Sample : N4579-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CHERRY-HILL-COMP-12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.197	319	325	331	rVB	25021	40065	2.05%	0.378%
2	5.679	399	407	419	rBV	484335	807100	41.34%	7.606%
3	7.288	674	681	697	rBV	470713	837579	42.90%	7.893%
4	8.135	818	825	835	rBB	146827	249558	12.78%	2.352%
5	9.310	1017	1025	1035	rBV	286341	521349	26.71%	4.913%
6	10.708	1256	1263	1283	rBV	130056	248019	12.70%	2.337%
7	10.961	1299	1306	1314	rVB	194564	355714	18.22%	3.352%
8	13.393	1712	1720	1732	rBV	850077	1337868	68.53%	12.607%
9	13.640	1756	1762	1769	rBV2	12036	19833	1.02%	0.187%
10	14.768	1948	1954	1967	rVB	324708	516850	26.48%	4.870%
11	16.260	2201	2208	2222	rBV	629392	1033566	52.94%	9.740%
12	16.454	2235	2241	2250	rVB	30438	50890	2.61%	0.480%
13	17.518	2415	2422	2430	rBV	414956	636280	32.59%	5.996%
14	18.152	2525	2530	2537	rVB	35275	44516	2.28%	0.419%
15	19.321	2721	2729	2732	rBV2	30372	41388	2.12%	0.390%
16	19.609	2774	2778	2783	rVB2	15310	19880	1.02%	0.187%
17	20.115	2859	2864	2877	rVB	1470167	1952194	100.00%	18.396%
18	20.896	2993	2997	3000	rBV	25316	30567	1.57%	0.288%
19	21.413	3080	3085	3098	rBV2	61852	129066	6.61%	1.216%
20	21.813	3146	3153	3160	rBV	417580	729766	37.38%	6.877%
21	21.971	3175	3180	3186	rVB	41769	61363	3.14%	0.578%
22	22.600	3283	3287	3292	rVB	36934	54706	2.80%	0.516%
23	23.323	3405	3410	3417	rVB3	28061	53636	2.75%	0.505%
24	24.163	3548	3553	3561	rVB3	25967	59946	3.07%	0.565%
25	25.179	3716	3726	3739	rVB2	250216	780168	39.96%	7.352%




Sum of corrected areas: 10611867

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
Data File : BG054937.D
Acq On : 14 Sep 2022 1:19
Operator : CG/JU
Sample : N4579-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

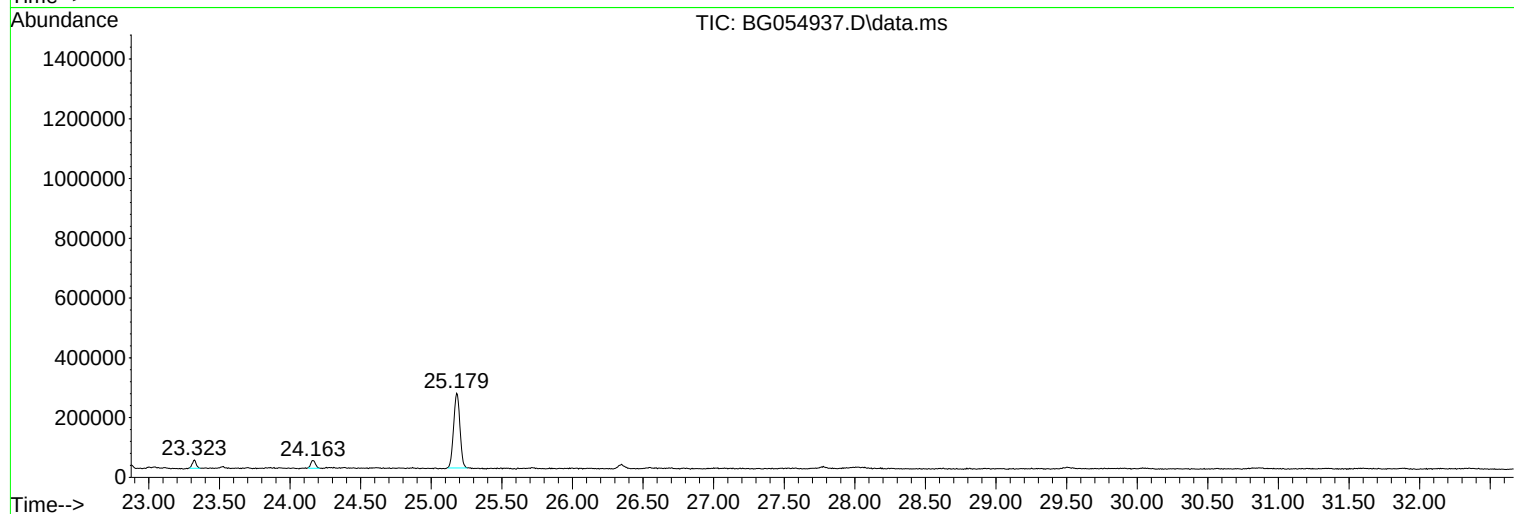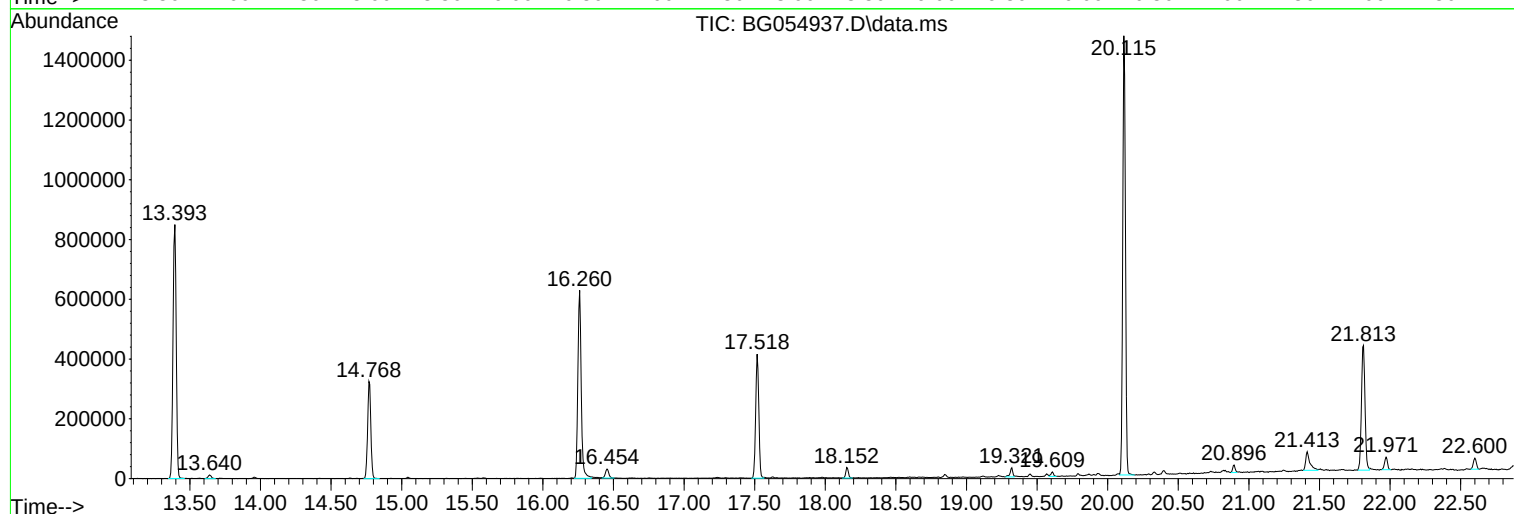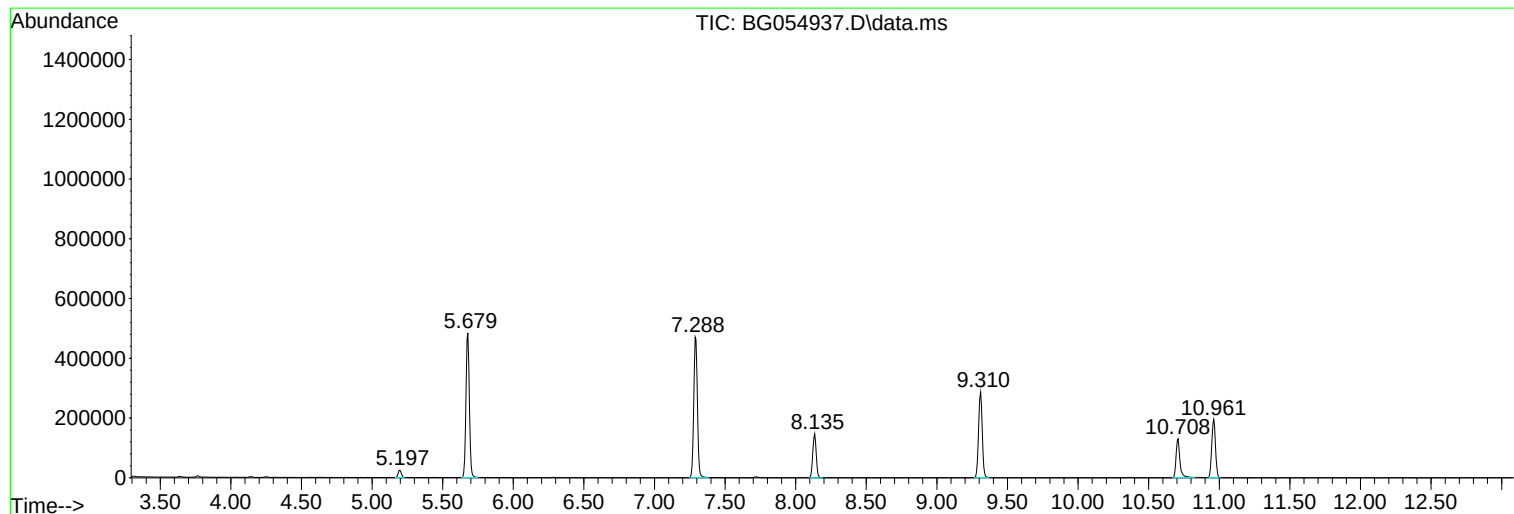

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
Data File : BG054937.D
Acq On : 14 Sep 2022 1:19
Operator : CG/JU
Sample : N4579-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
Data File : BG054937.D
Acq On : 14 Sep 2022 1:19
Operator : CG/JU
Sample : N4579-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc