
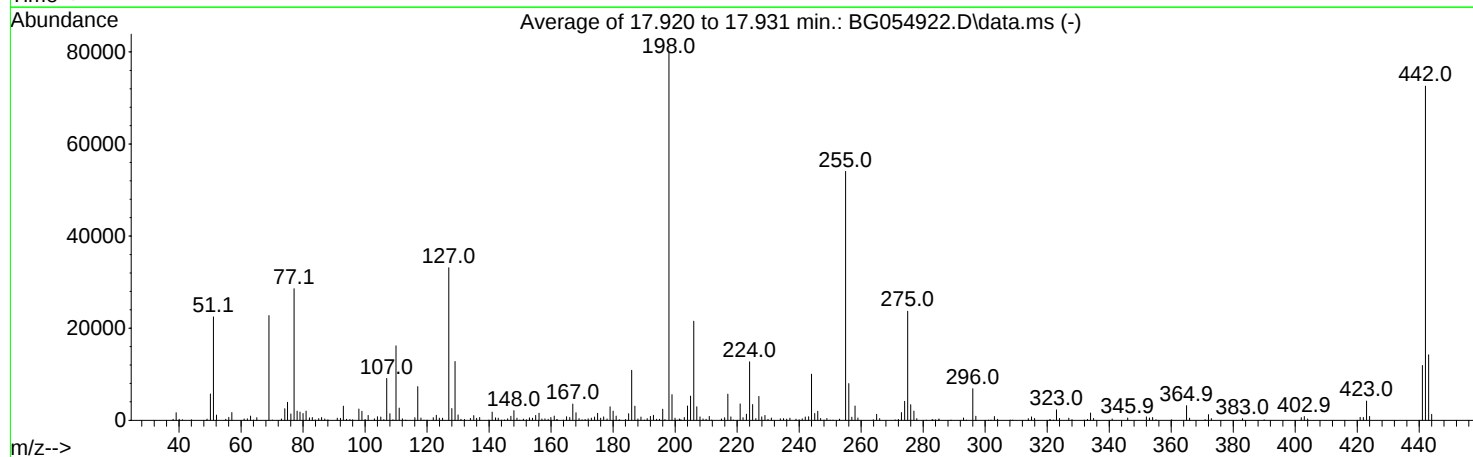


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
 Data File : BG054922.D
 Acq On : 13 Sep 2022 13:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 10 01:53:42 2022

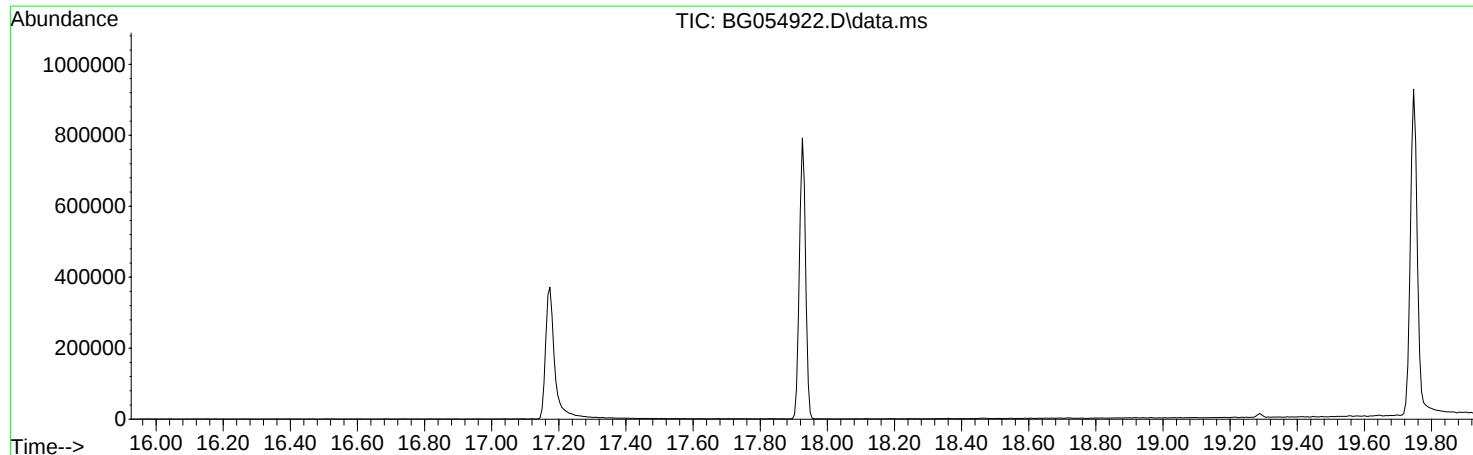




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	22475	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.5	22763	PASS
70	69	0.00	2	0.2	51	PASS
127	198	10	80	41.5	33149	PASS
197	198	0.00	2	0.2	155	PASS
198	198	100	100	100.0	79893	PASS
199	198	5	9	7.0	5579	PASS
275	198	10	60	29.7	23693	PASS
365	198	1	100	4.0	3197	PASS
441	198	0.01	100	14.9	11904	PASS
442	442	50	100	100.0	72573	PASS
443	442	15	24	19.6	14245	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
Data File : BG054922.D
Acq On : 13 Sep 2022 13:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 13 14:36:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

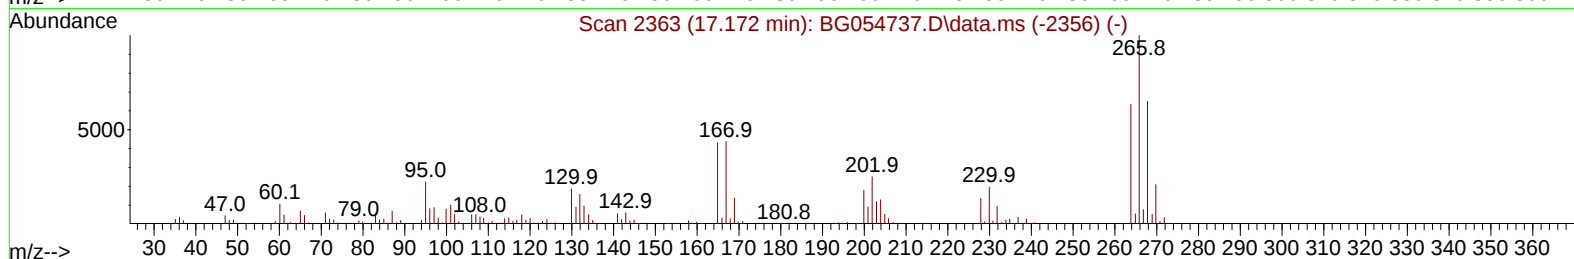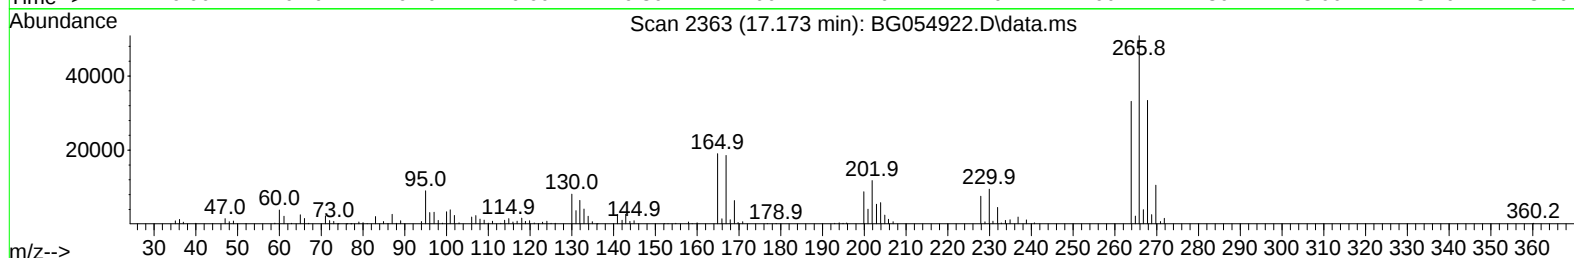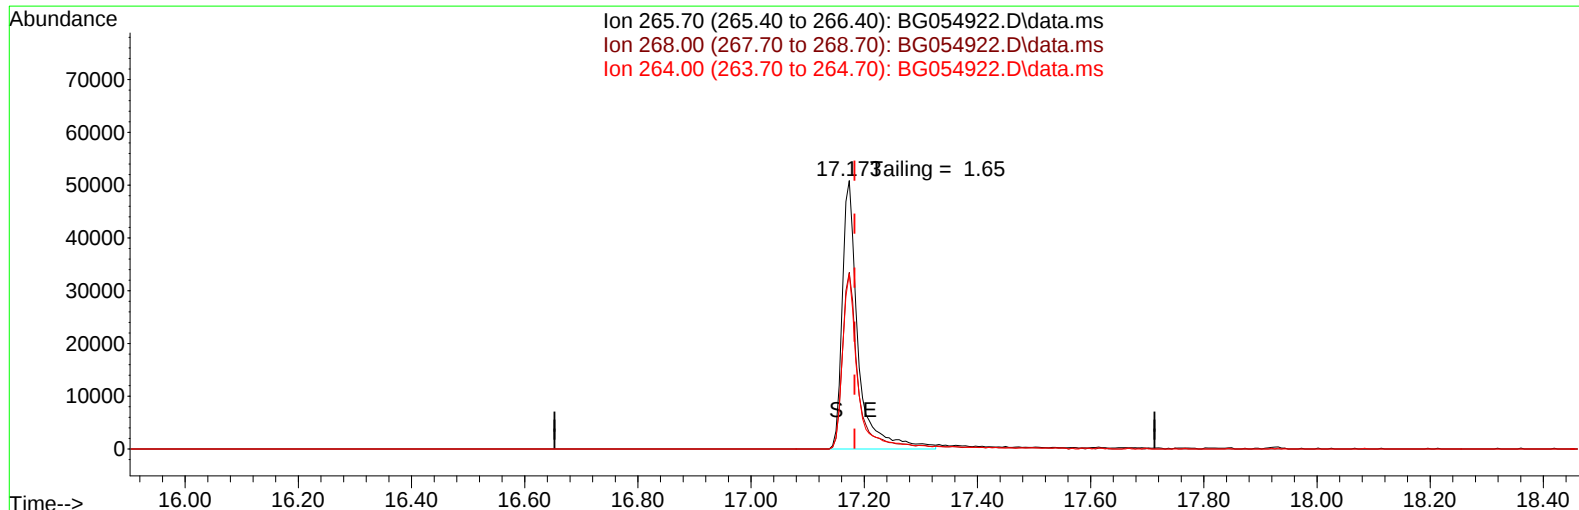

TIC: BG054922.D\data.ms

(70) Pentachlorophenol (C)

17.173min (-0.009) 38414.62 ng




response 99438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.75
264.00	61.70	65.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091322\
 Data File : BG054922.D
 Acq On : 13 Sep 2022 13:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 14:36:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 10 01:53:42 2022
 Response via : Initial Calibration

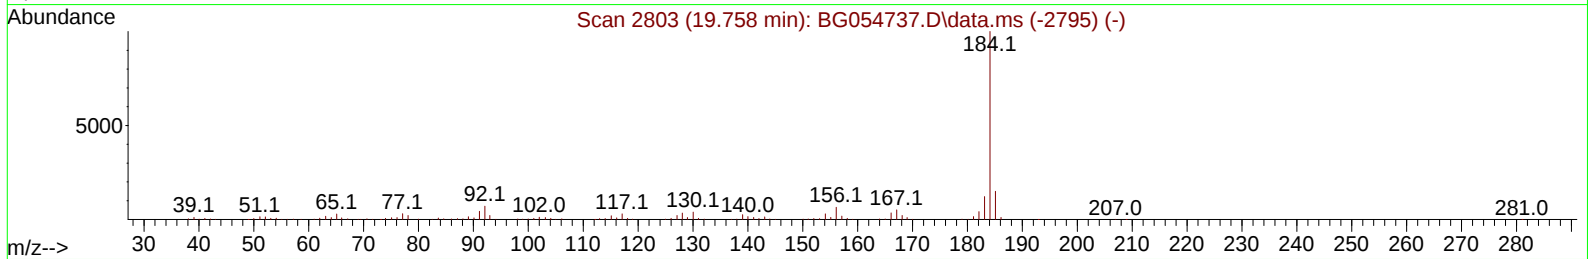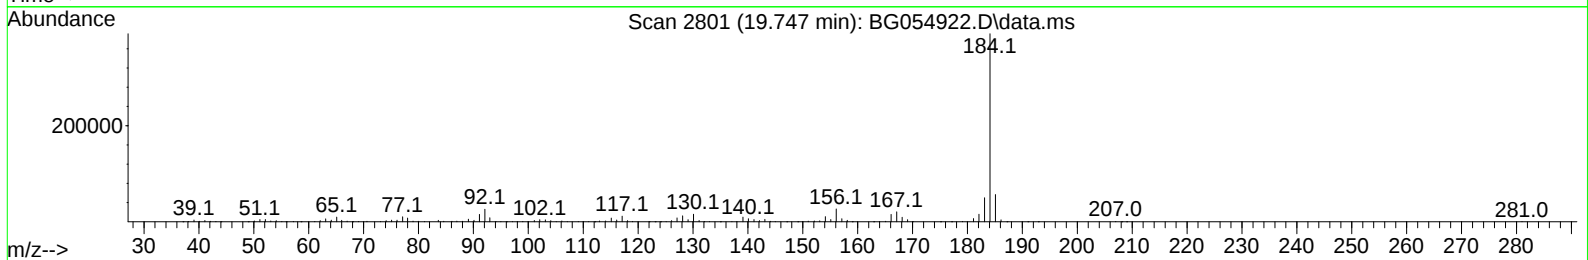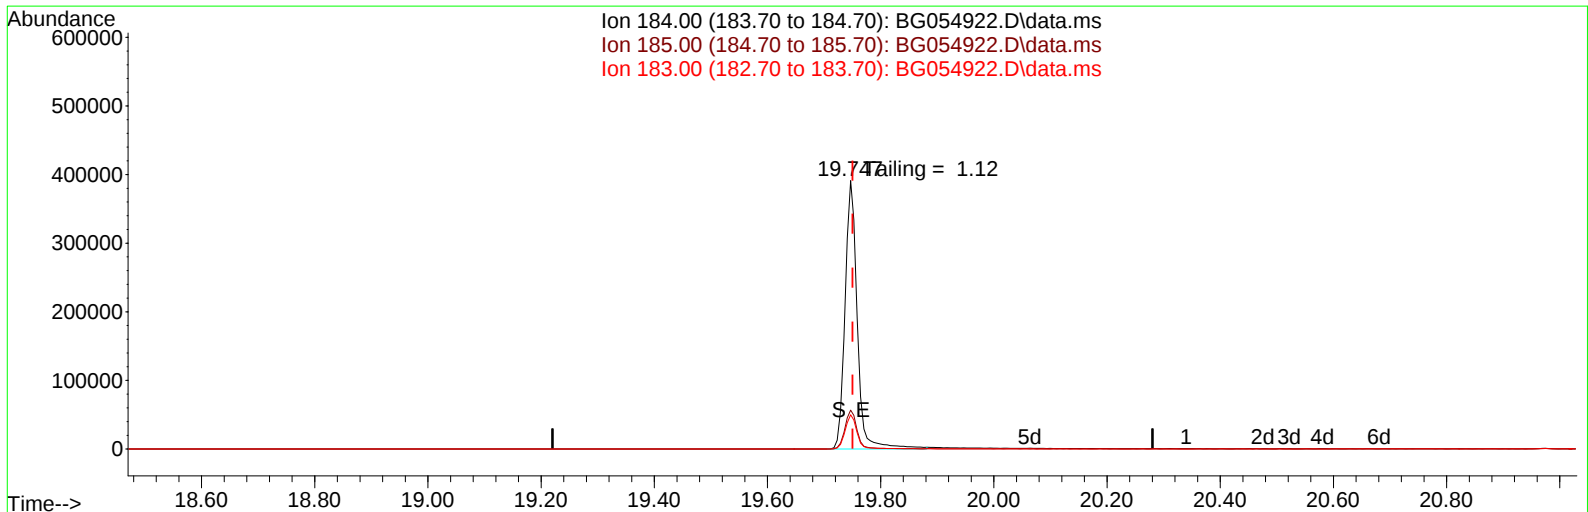

TIC: BG054922.D\data.ms

(77) Benzidine

19.747min (-0.003) 447789.20 ng m

response 587833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.51
183.00	12.30	12.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2022	BNA_G	BG054922.D
Compound Name	Response	Retention Time
DDT	290033	20.975
DDD	7181	20.528
DDE	668	20.023
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7849	297882	2.63

Instrument :
BNA_G
ClientSampleId :
DFTPP