




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062859.D
Acq On : 16 Sep 2024 00:05
Operator : JU/RC
Sample : PB163396BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK396

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:27:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

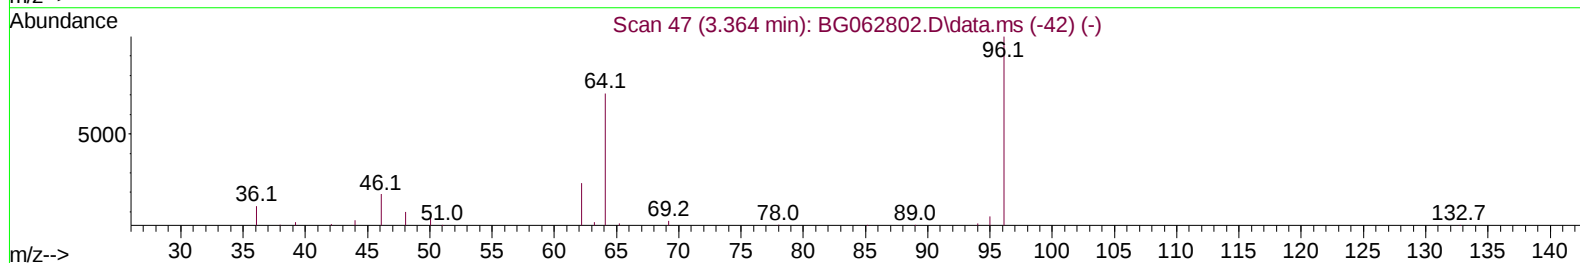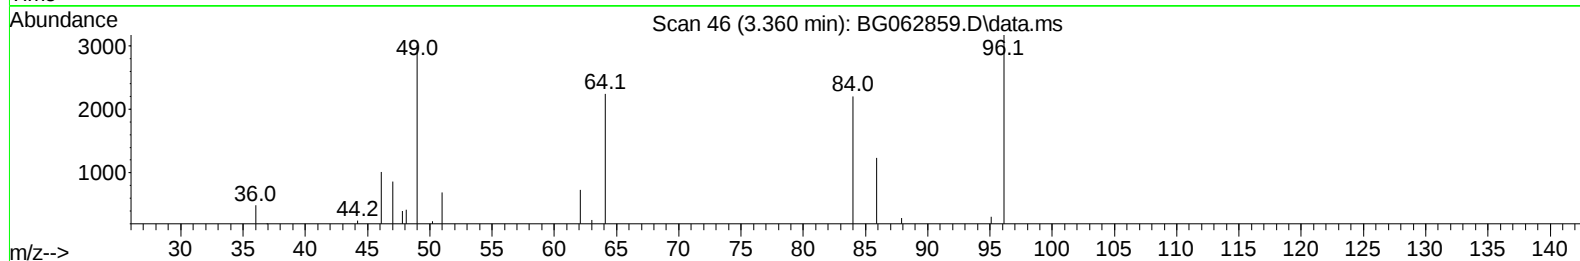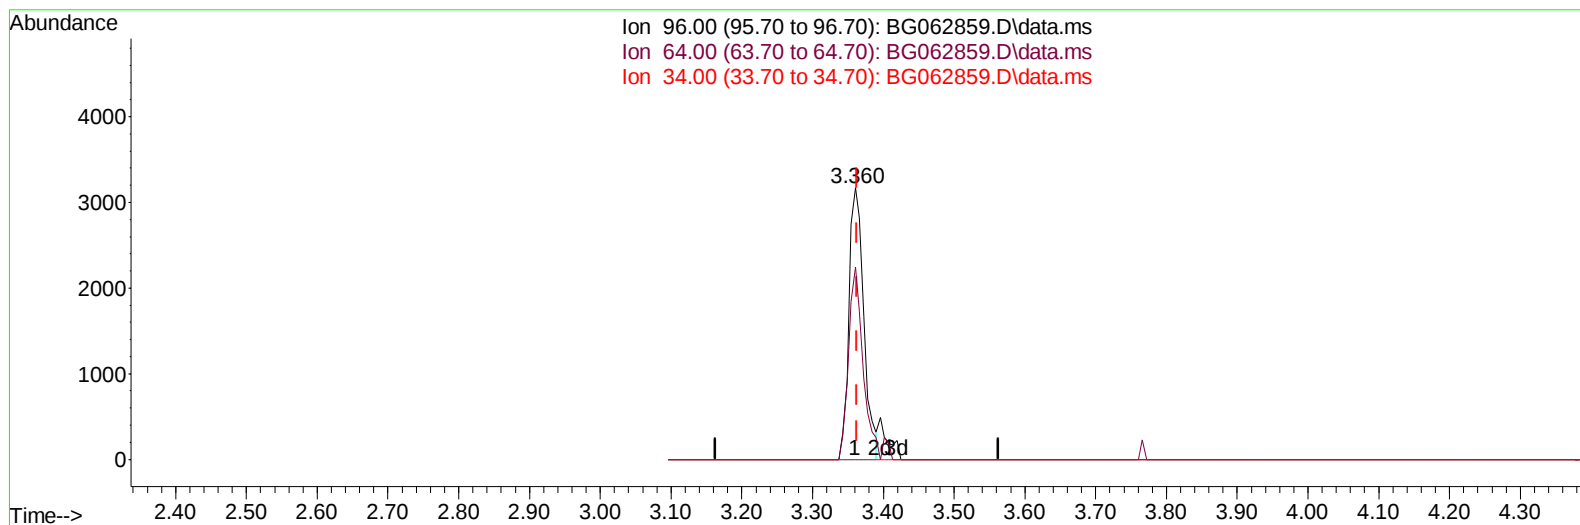

TIC: BG062859.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.360min (-0.003) 5.62 ng/uL

response 4616

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.00	70.87
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062859.D
Acq On : 16 Sep 2024 00:05
Operator : JU/RC
Sample : PB163396BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK396

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:27:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

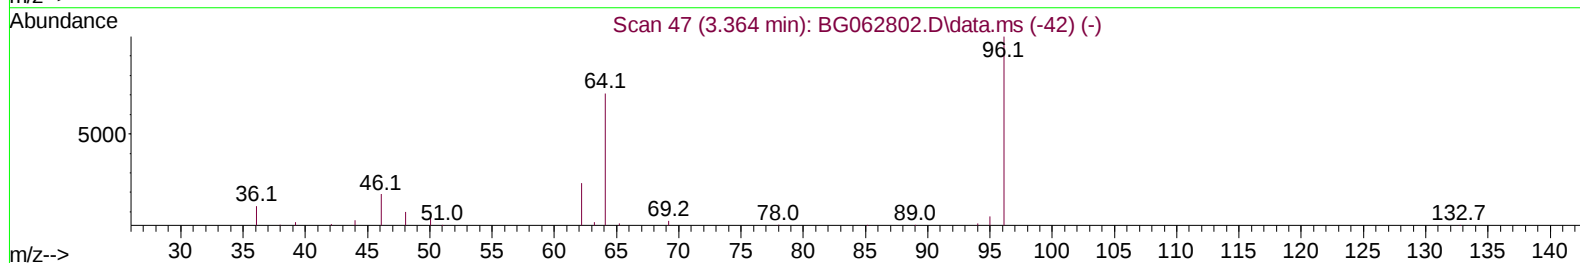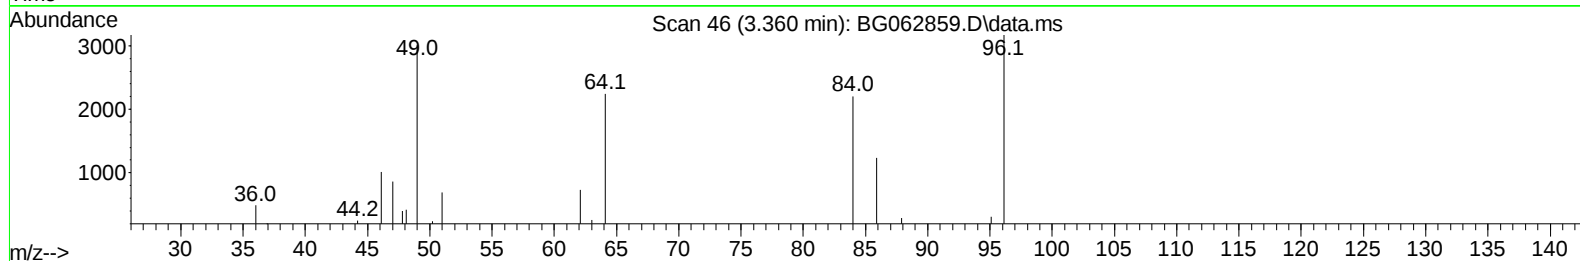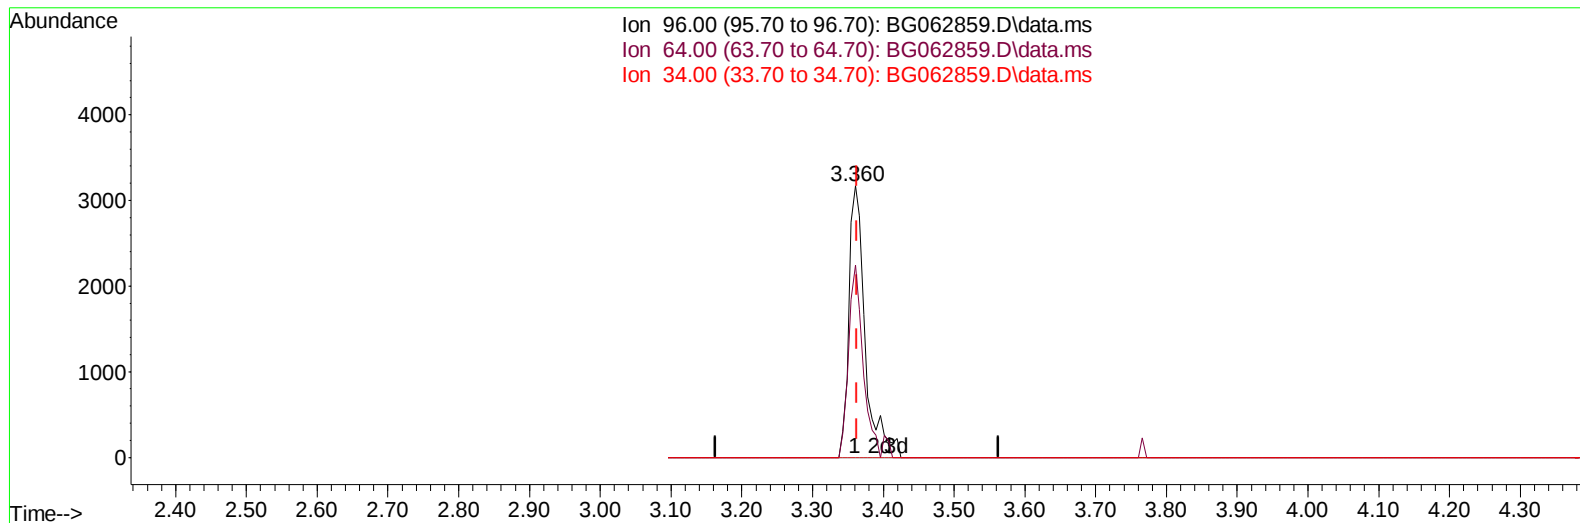

TIC: BG062859.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.360min (-0.003) 6.18 ng/uL m

response 5082

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.00	70.87
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062859.D
 Acq On : 16 Sep 2024 00:05
 Operator : JU/RC
 Sample : PB163396BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK396

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 01:29:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.902	152	37149	20.000	ng/ul	0.00
20) Naphthalene-d8	10.693	136	146201	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.530	164	128159	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.274	188	358513	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.522	240	404402	20.000	ng/ul	# 0.00
88) Perylene-d12	24.583	264	457866	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	5082m	6.184	ng/uL	0.00
4) Pyridine-d5	3.766	84	67563	25.827	ng/ul	0.00
7) Phenol-d5	7.068	99	85838	26.351	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.226	67	49958	25.580	ng/ul	0.00
11) 2-Chlorophenol-d4	7.432	132	66660	28.094	ng/ul	0.00
15) 4-Methylphenol-d8	8.607	113	78233	28.819	ng/ul	0.00
21) Nitrobenzene-d5	9.054	128	35923	34.379	ng/ul	0.00
24) 2-Nitrophenol-d4	9.776	143	42630	37.304	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.317	165	83154	33.413	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	97494	28.500	ng/ul	0.00
46) Dimethylphthalate-d6	13.930	166	307492	31.157	ng/ul	0.00
49) Acenaphthylene-d8	14.218	160	334273	30.497	ng/ul	0.00
54) 4-Nitrophenol-d4	14.729	143	48474	28.913	ng/ul	0.00
60) Fluorene-d10	15.523	176	289485	32.551	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.640	200	62627	30.368	ng/ul	0.00
73) Anthracene-d10	17.373	188	550115	32.513	ng/ul	0.00
81) Pyrene-d10	19.665	212	717562	31.532	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.377	264	763526	31.581	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062859.D
Acq On : 16 Sep 2024 00:05
Operator : JU/RC
Sample : PB163396BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK396

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:29:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

